

#17

Hexachloroethane

Concen: 19.163 ng/ul

RT: 8.65 min Scan# 963

Delta R.T. 0.00 min

Lab File: BN005416.D

Acq: 02 May 2019 15:34

Instrument :

BNA_N

ClientSampleId :


Tgt Ion:117 Resp: 137794

Ion Ratio Lower Upper

117 100

201 114.5 84.1 126.1




199 71.1 51.2 76.8

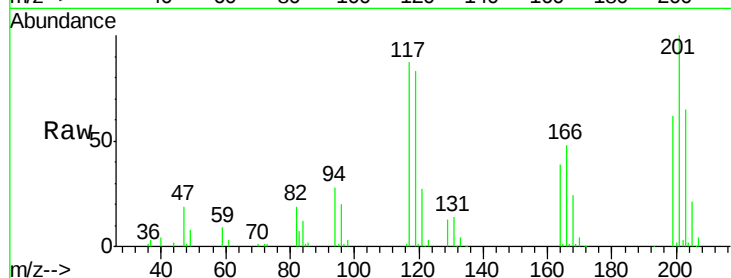

Abundance Ion 117.00 (116.70 to 117.70): E

Ion 201.00 (200.70 to 201.70): E

Ion 199.00 (198.70 to 199.70): E

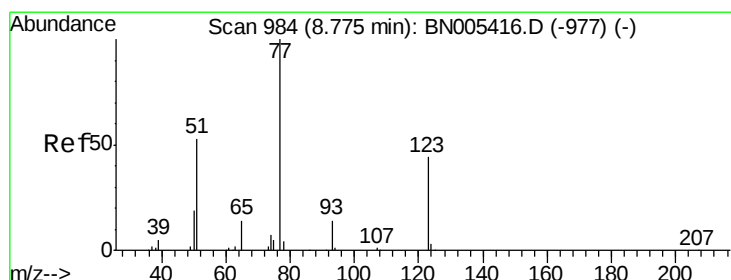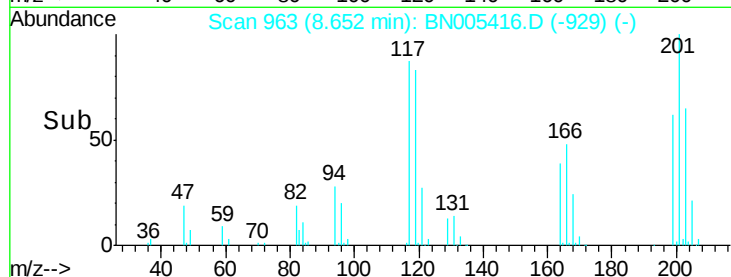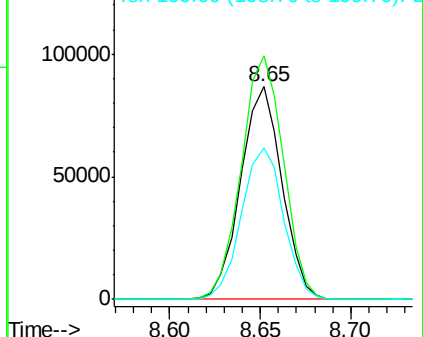

#20

Nitrobenzene

Concen: 20.033 ng/ul

RT: 8.78 min Scan# 984

Delta R.T. 0.00 min

Lab File: BN005416.D

Acq: 02 May 2019 15:34


Tgt Ion: 77 Resp: 389867

Ion Ratio Lower Upper

77 100

123 43.8 32.6 49.0

65 13.9 11.6 17.4

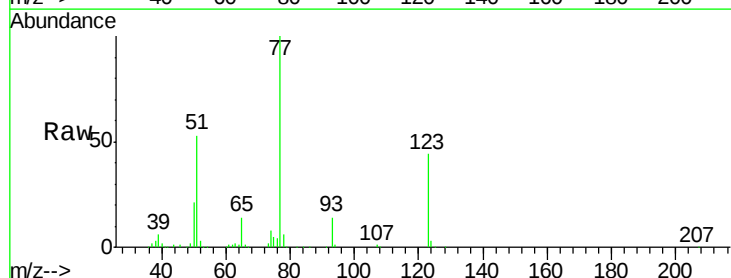

Abundance Ion 77.00 (76.70 to 77.70): BNC

Ion 123.00 (122.70 to 123.70): E

Ion 65.00 (64.70 to 65.70): BNC

