

#37

Hexachlorocyclopentadiene

Concen: 19.985 ng/ul

RT: 12.38 min Scan# 1596

Delta R.T. 0.00 min

Lab File: BN005416.D

Acq: 02 May 2019 15:34

Instrument :

BNA\_N

ClientSampled :


Tgt Ion:237 Resp: 313233

Ion Ratio Lower Upper

237 100

235 64.3 51.1 76.7




272 12.3 9.5 14.3

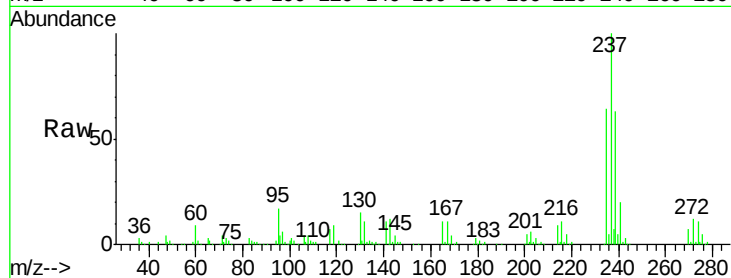

Abundance Ion 237.00 (236.70 to 237.70): E

Ion 235.00 (234.70 to 235.70): E

Ion 272.00 (271.70 to 272.70): E

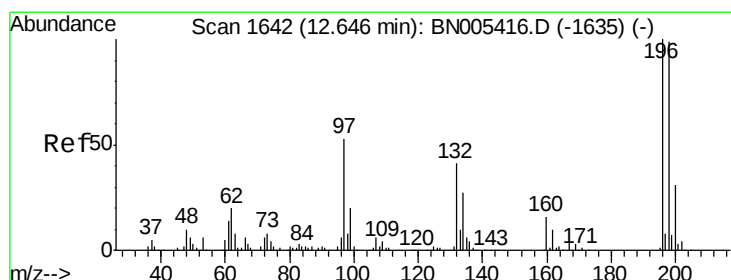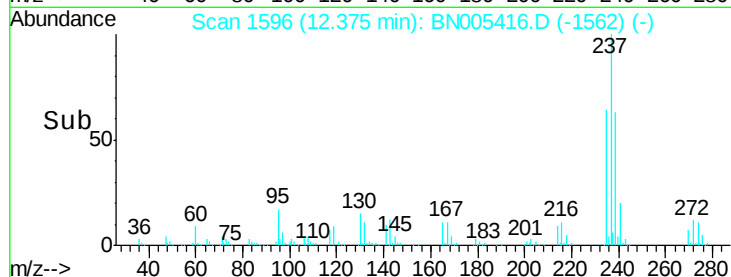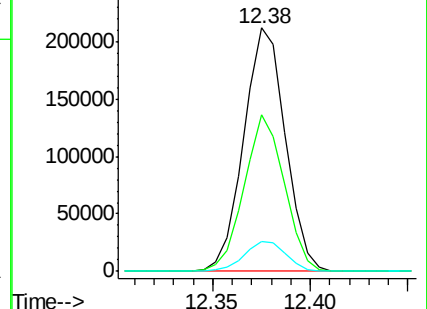

#38

2,4,6-Trichlorophenol

Concen: 21.932 ng/ul

RT: 12.65 min Scan# 1642

Delta R.T. 0.00 min

Lab File: BN005416.D

Acq: 02 May 2019 15:34


Tgt Ion:196 Resp: 304011

Ion Ratio Lower Upper

196 100

198 99.0 74.8 112.2

200 30.5 23.5 35.3

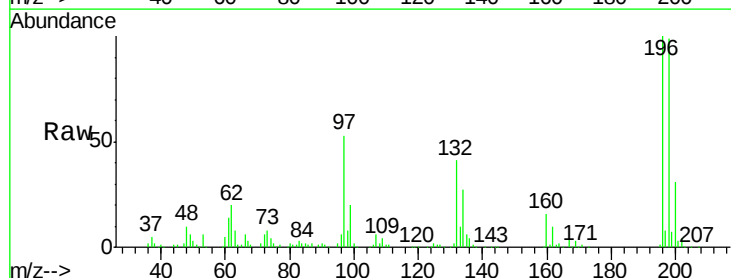

Abundance Ion 196.00 (195.70 to 196.70): E

Ion 198.00 (197.70 to 198.70): E

Ion 200.00 (199.70 to 200.70): E

