
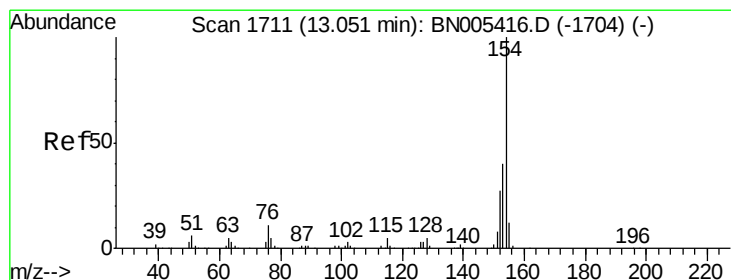
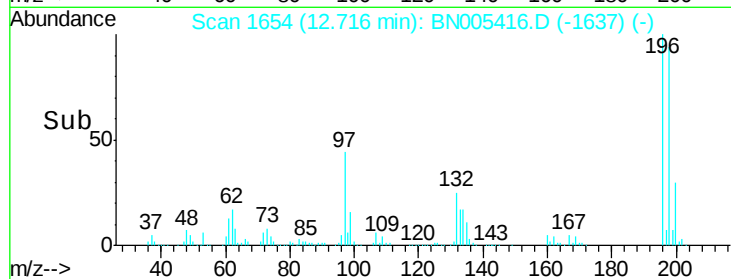
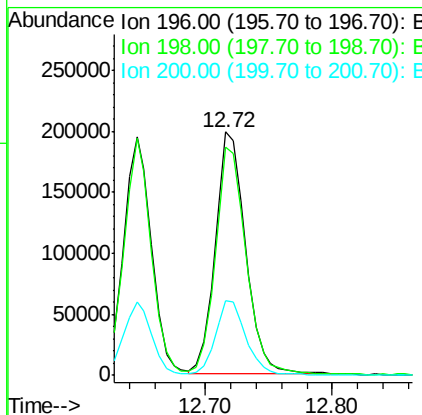


#39
 2,4,5-Trichlorophenol
 Concen: 22.156 ng/ul
 RT: 12.72 min Scan# 1654
 Delta R.T. 0.00 min
 Lab File: BN005416.D
 Acq: 02 May 2019 15:34

Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion:196 Resp: 330015
 Ion Ratio Lower Upper
 196 100
 198 93.8 75.0 112.4
 200 30.4 24.2 36.4

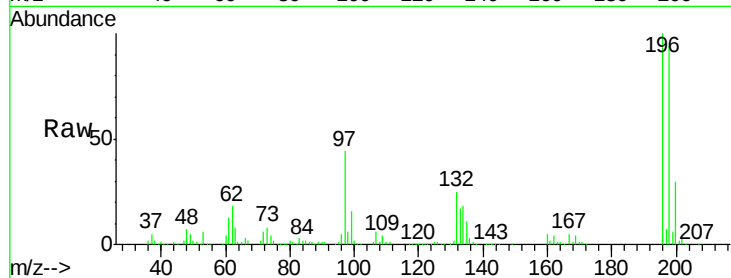

#40
 1,1'-Biphenyl
 Concen: 19.884 ng/ul
 RT: 13.05 min Scan# 1711
 Delta R.T. 0.00 min
 Lab File: BN005416.D
 Acq: 02 May 2019 15:34

Tgt Ion:154 Resp: 1100494
 Ion Ratio Lower Upper
 154 100
 153 40.0 32.6 49.0
 76 11.4 10.4 15.6

