





#41
 2-Chloronaphthalene
 Concen: 19.836 ng/ul
 RT: 13.09 min Scan# 1718
 Delta R.T. 0.00 min
 Lab File: BN005416.D
 Acq: 02 May 2019 15:34

Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion	Ratio	Lower	Upper
162	100		
164	32.8	26.8	40.2
127	38.7	33.5	50.3

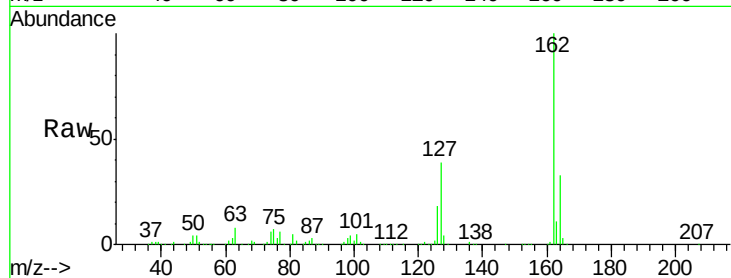


Abundance Ion 162.00 (161.70 to 162.70): E
 Ion 164.00 (163.70 to 164.70): E
 Ion 127.00 (126.70 to 127.70): E

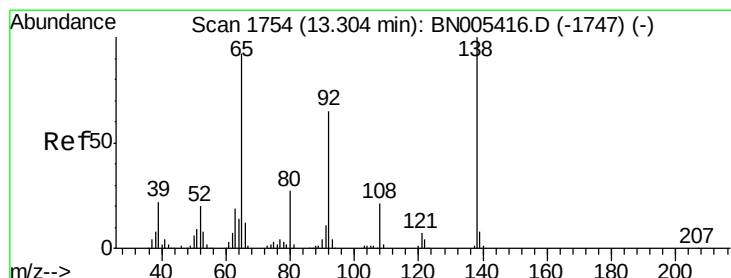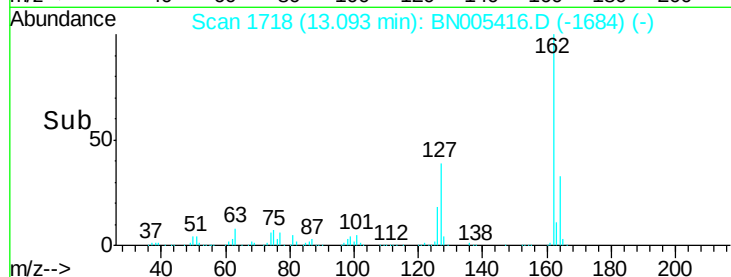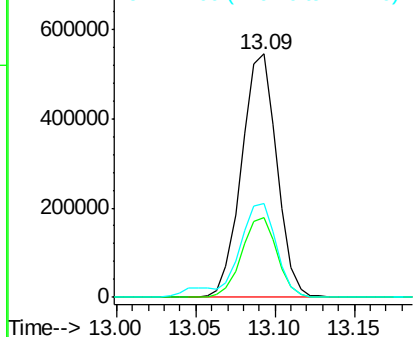

#42
 2-Nitroaniline
 Concen: 22.365 ng/ul
 RT: 13.30 min Scan# 1754
 Delta R.T. 0.00 min
 Lab File: BN005416.D
 Acq: 02 May 2019 15:34

Tgt Ion	Ratio	Lower	Upper
65	100		
92	70.7	51.6	77.4
138	109.0	73.9	110.9

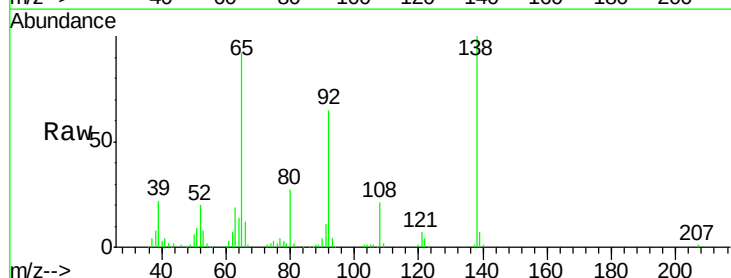

Abundance Ion 65.00 (64.70 to 65.70): BNC
 Ion 92.00 (91.70 to 92.70): BNC
 Ion 138.00 (137.70 to 138.70): E

