
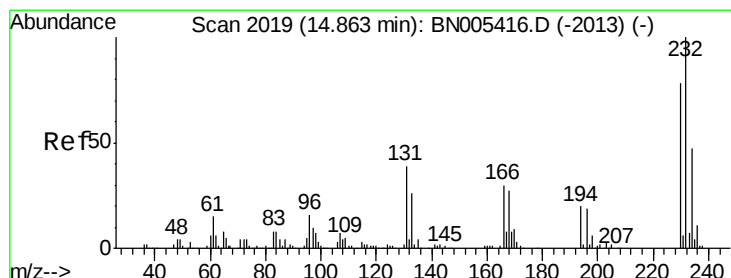
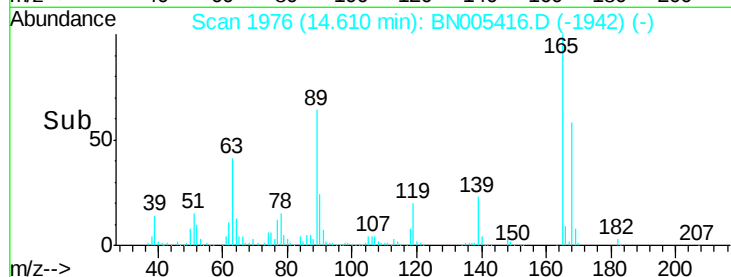
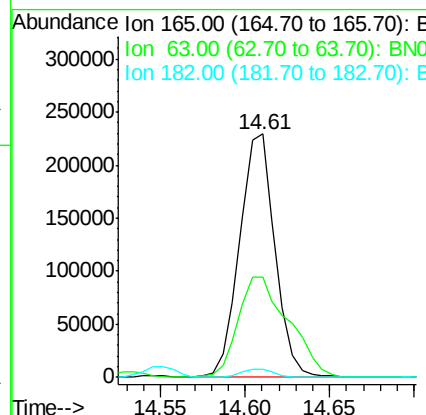


#54
 2,4-Dinitrotoluene
 Concen: 25.043 ng/ul
 RT: 14.61 min Scan# 1976
 Delta R.T. 0.00 min
 Lab File: BN005416.D
 Acq: 02 May 2019 15:34

Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion:165 Resp: 334925
 Ion Ratio Lower Upper
 165 100
 63 41.1 38.9 58.3
 182 3.3 2.6 3.8

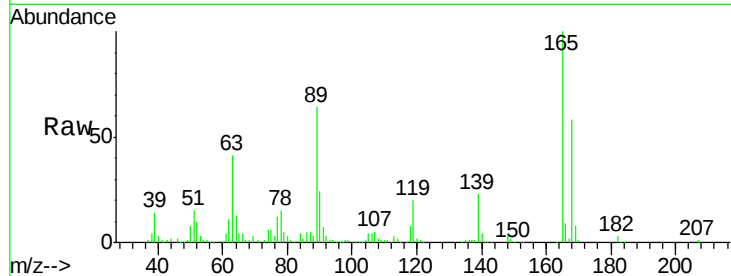

#55
 2,3,4,6-Tetrachlorophenol
 Concen: 23.860 ng/ul
 RT: 14.86 min Scan# 2019
 Delta R.T. 0.00 min
 Lab File: BN005416.D
 Acq: 02 May 2019 15:34

Tgt Ion:232 Resp: 295661
 Ion Ratio Lower Upper
 232 100
 131 38.6 36.6 54.8
 130 2.2 2.0 3.0
 166 29.7 26.6 39.8

