
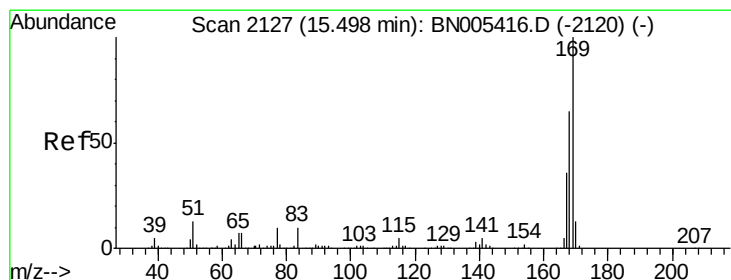
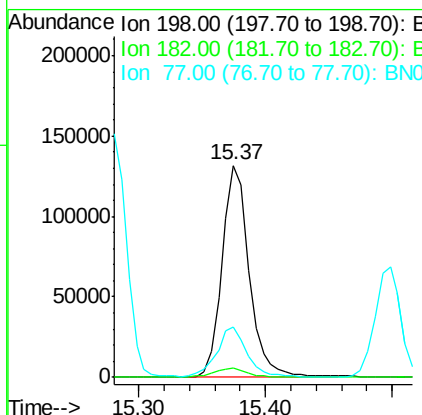
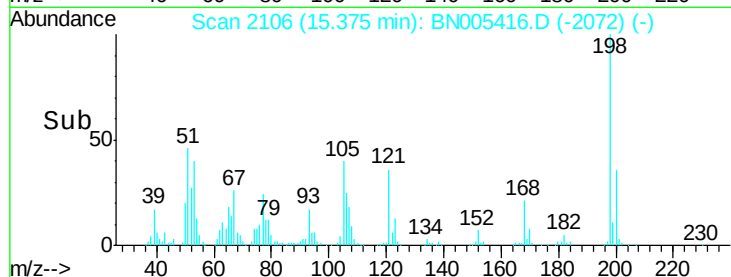


#63
 4,6-Dinitro-2-methylphenol
 Concen: 23.292 ng/ul
 RT: 15.37 min Scan# 2106
 Delta R.T. 0.00 min
 Lab File: BN005416.D
 Acq: 02 May 2019 15:34

Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion:198 Resp: 196324
 Ion Ratio Lower Upper
 198 100
 182 4.6 3.0 4.6
 77 23.6 21.9 32.9

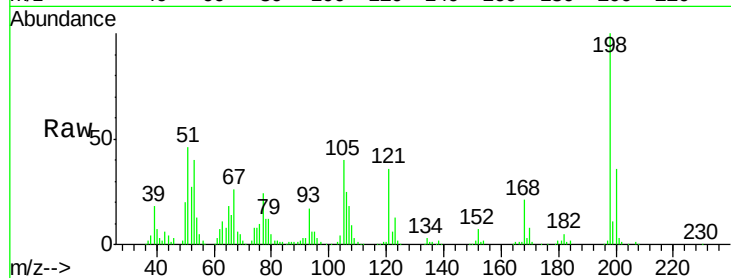

#64
 N-Nitrosodiphenylamine
 Concen: 19.867 ng/ul
 RT: 15.50 min Scan# 2127
 Delta R.T. 0.00 min
 Lab File: BN005416.D
 Acq: 02 May 2019 15:34

Tgt Ion:169 Resp: 957431
 Ion Ratio Lower Upper
 169 100
 168 65.2 52.2 78.2
 167 35.8 27.7 41.5

