





#65
 4-Bromophenyl-phenylether
 Concen: 20.600 ng/ul
 RT: 16.18 min Scan# 2243
 Delta R.T. 0.00 min
 Lab File: BN005416.D
 Acq: 02 May 2019 15:34

Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion:248 Resp: 365423
 Ion Ratio Lower Upper
 248 100
 250 97.4 78.4 117.6
 141 65.7 61.8 92.6

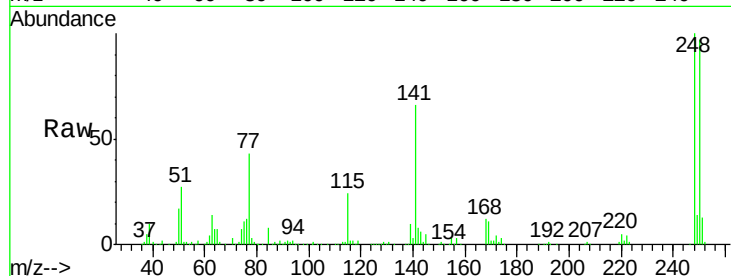


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

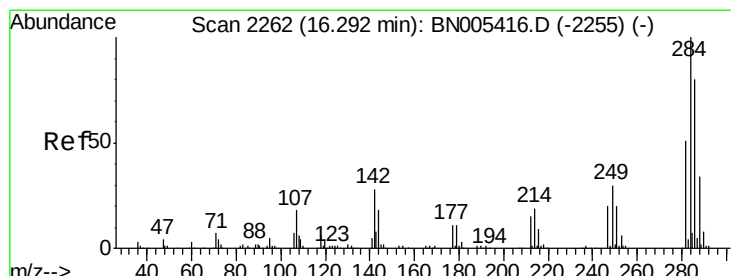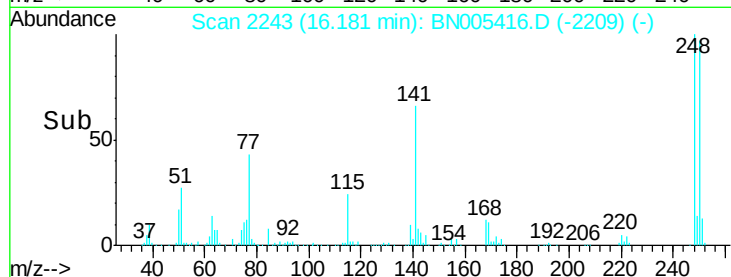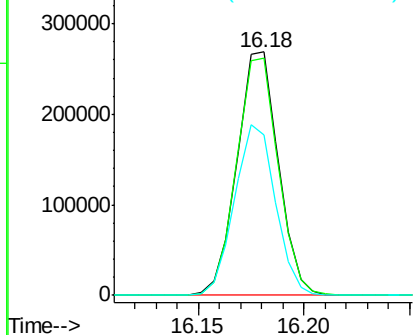

#66
 Hexachlorobenzene
 Concen: 21.363 ng/ul
 RT: 16.29 min Scan# 2262
 Delta R.T. 0.00 min
 Lab File: BN005416.D
 Acq: 02 May 2019 15:34

Tgt Ion:284 Resp: 403535
 Ion Ratio Lower Upper
 284 100
 142 27.7 29.4 44.2#
 249 29.6 26.1 39.1

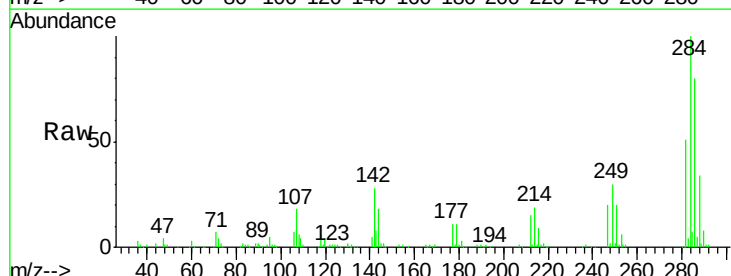

Abundance Ion 284.00 (283.70 to 284.70): E
 Ion 142.00 (141.70 to 142.70): E
 Ion 249.00 (248.70 to 249.70): E

