

#67

Atrazine

Concen: 20.861 ng/ul

RT: 16.46 min Scan# 2290

Delta R.T. 0.00 min

Lab File: BN005416.D

Acq: 02 May 2019 15:34

Instrument :

BNA_N

ClientSampleId :


Tgt Ion:200 Resp: 374277

Ion Ratio Lower Upper

200 100

173 25.6 21.4 32.0




215 51.1 39.1 58.7

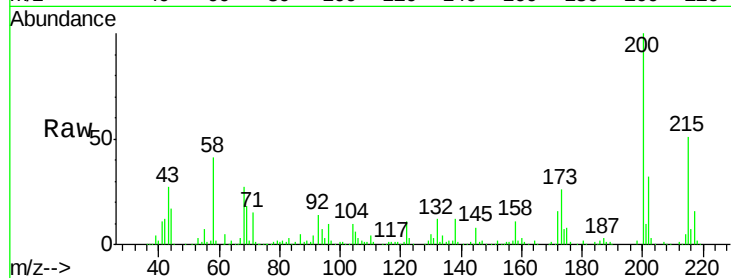

Abundance Ion 200.00 (199.70 to 200.70): E

Ion 173.00 (172.70 to 173.70): E

Ion 215.00 (214.70 to 215.70): E

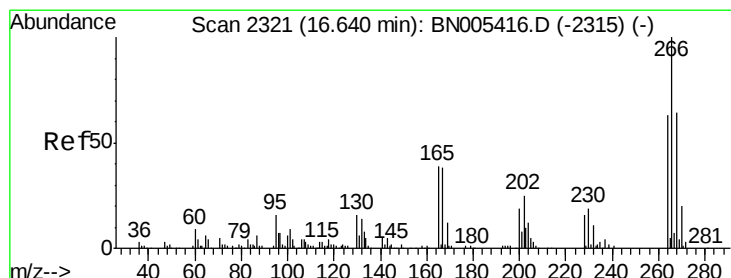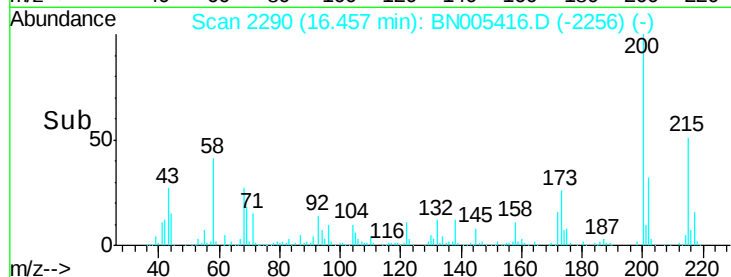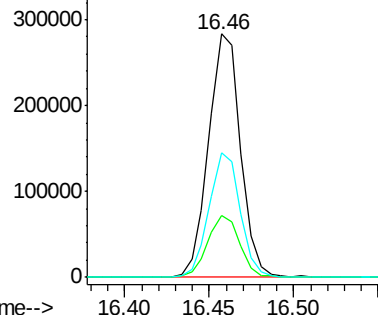

#68

Pentachlorophenol

Concen: 20.474 ng/ul

RT: 16.64 min Scan# 2321

Delta R.T. 0.00 min

Lab File: BN005416.D

Acq: 02 May 2019 15:34


Tgt Ion:266 Resp: 226444

Ion Ratio Lower Upper

266 100

264 63.0 49.7 74.5

268 63.8 52.4 78.6

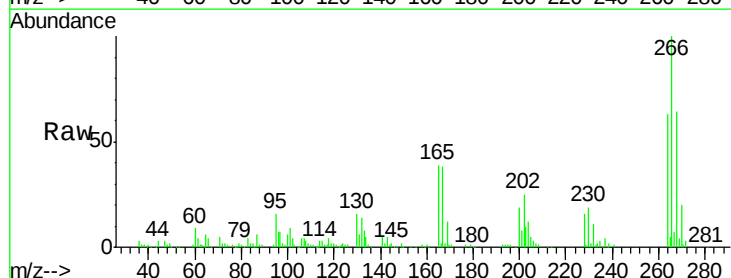

Abundance Ion 265.70 (265.40 to 266.40): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

