
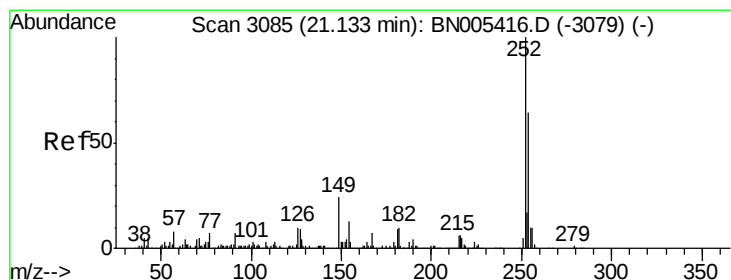
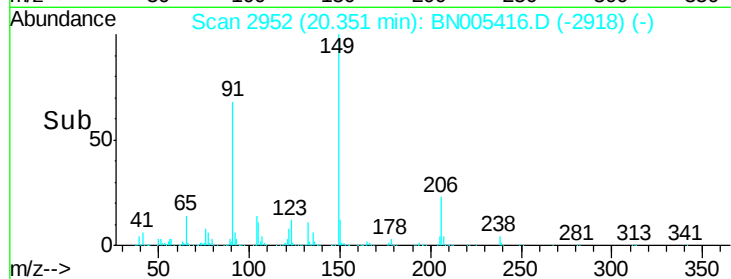
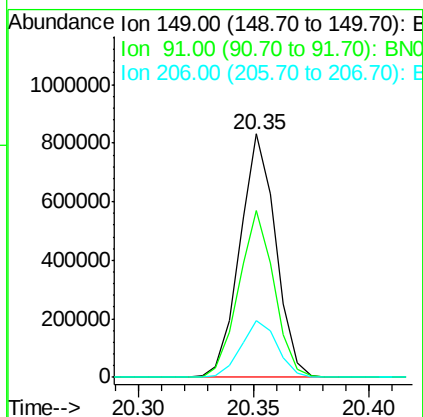


#80
Butylbenzylphthalate
Concen: 20.163 ng/ul
RT: 20.35 min Scan# 2952
Delta R.T. 0.00 min
Lab File: BN005416.D
Acq: 02 May 2019 15:34

Instrument :
BNA_N
ClientSampleId :

Tgt Ion	Ratio	Lower	Upper
149	100		
91	68.3	59.6	89.4
206	23.4	17.8	26.8

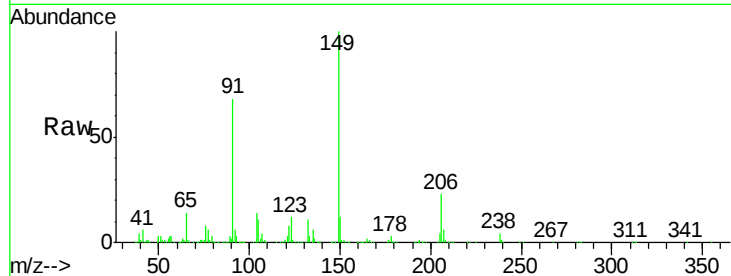

#81
3,3'-Dichlorobenzidine
Concen: 20.048 ng/ul
RT: 21.13 min Scan# 3085
Delta R.T. 0.00 min
Lab File: BN005416.D
Acq: 02 May 2019 15:34

Tgt Ion	Ratio	Lower	Upper
252	100		
254	63.8	51.1	76.7
126	9.8	9.4	14.0

