

#82

Benzo(a)anthracene

Concen: 20.066 ng/ul

RT: 21.20 min Scan# 3096

Delta R.T. 0.00 min

Lab File: BN005416.D

Acq: 02 May 2019 15:34

Instrument :

BNA_N

ClientSampleId :


Tgt Ion:228 Resp: 2185083

Ion Ratio Lower Upper

228 100

229 19.9 15.8 23.6




226 26.6 21.4 32.2

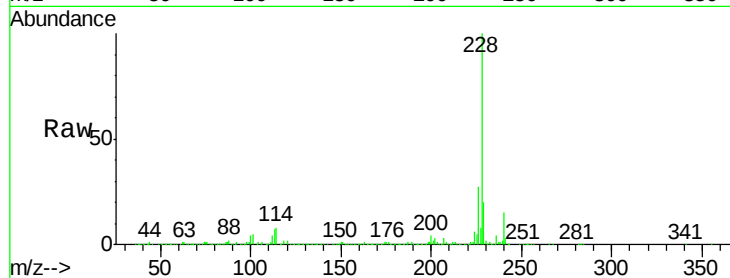

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

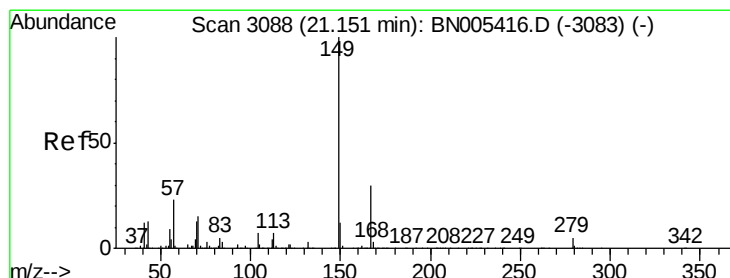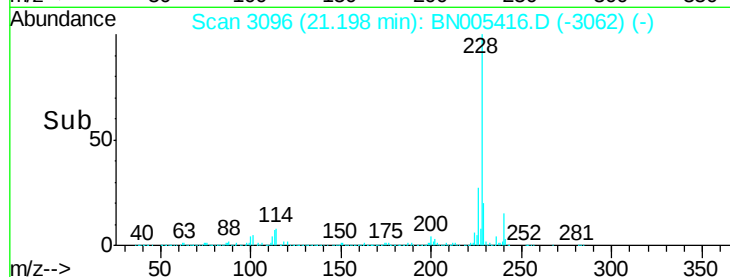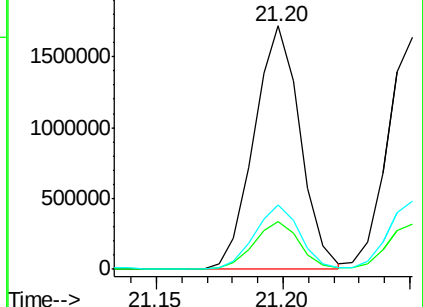

#83

Bis(2-ethylhexyl)phthalate

Concen: 19.251 ng/ul

RT: 21.15 min Scan# 3088

Delta R.T. 0.00 min

Lab File: BN005416.D

Acq: 02 May 2019 15:34


Tgt Ion:149 Resp: 1322788

Ion Ratio Lower Upper

149 100

167 30.0 22.3 33.5

279 5.5 3.3 4.9#

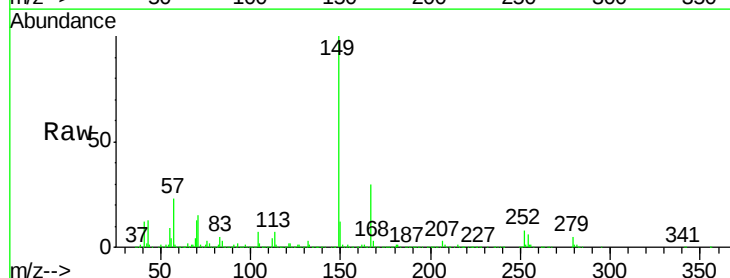

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

