

#84

Chrysene

Concen: 20.432 ng/ul

RT: 21.25 min Scan# 3105

Delta R.T. 0.00 min

Lab File: BN005416.D

Acq: 02 May 2019 15:34

Instrument :

BNA_N

ClientSampleId :


Tgt Ion:228 Resp: 2065026

Ion	Ratio	Lower	Upper
228	100		
226	29.6	24.0	36.0
229	19.7	15.4	23.0

228 100

226 29.6 24.0 36.0




229 19.7 15.4 23.0

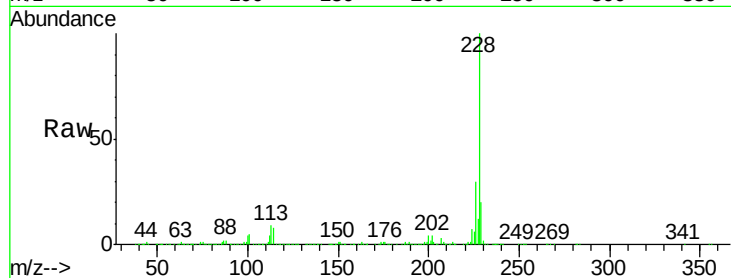

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

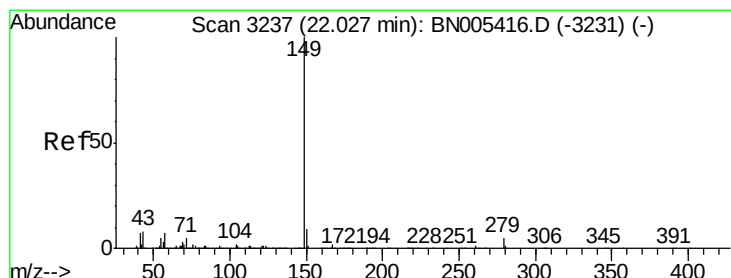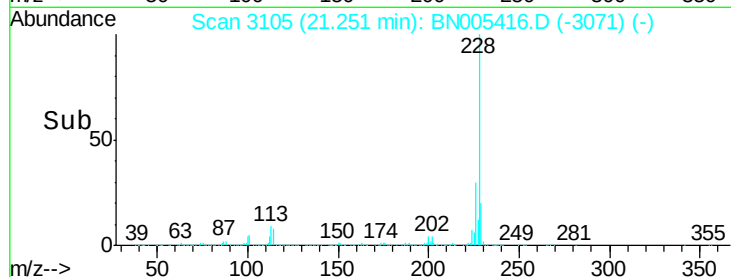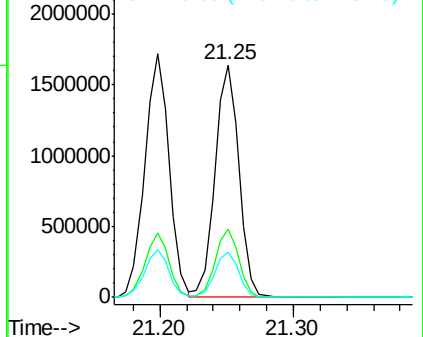

#86

Di-n-octyl phthalate

Concen: 21.102 ng/ul


RT: 22.03 min Scan# 3237

Delta R.T. 0.00 min

Lab File: BN005416.D

Acq: 02 May 2019 15:34

Tgt Ion:149 Resp: 2263174

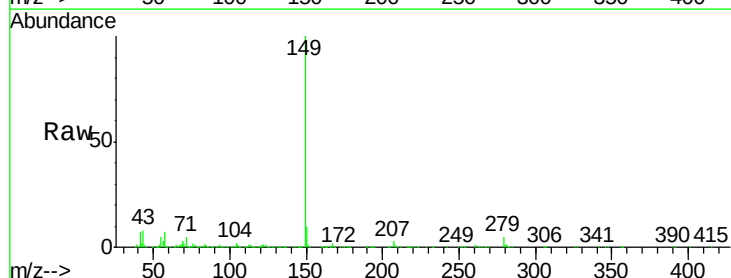

Abundance Ion 149.00 (148.70 to 149.70): E

