

#92

Dibenzo(a,h)anthracene

Concen: 18.751 ng/ul

RT: 25.62 min Scan# 3848

Delta R.T. 0.00 min

Lab File: BN005416.D

Acq: 02 May 2019 15:34

Instrument :

BNA_N

ClientSampleId :


Tgt Ion:278 Resp: 1627919

Ion Ratio Lower Upper

278 100

139 14.2 13.1 19.7




279 24.6 19.4 29.0

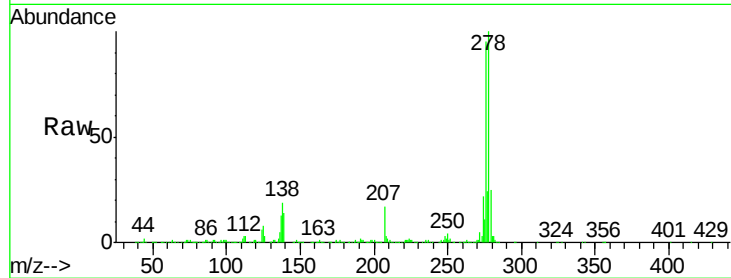

Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

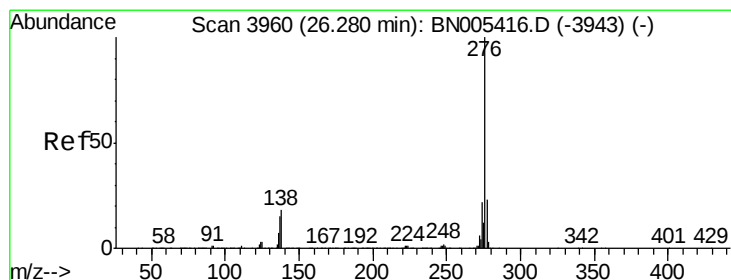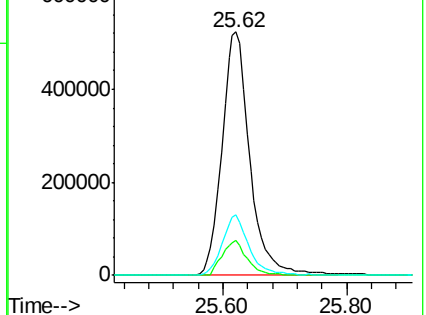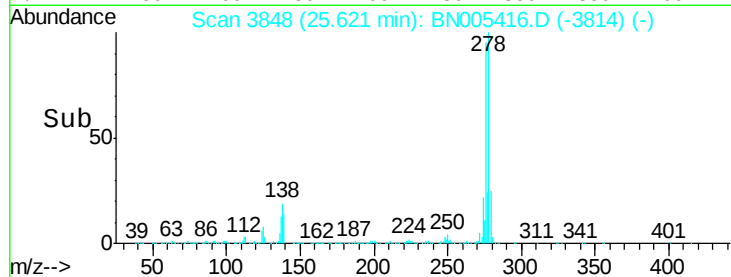

#93

Benzo(g,h,i)perylene

Concen: 18.466 ng/ul

RT: 26.28 min Scan# 3960

Delta R.T. 0.00 min

Lab File: BN005416.D

Acq: 02 May 2019 15:34


Tgt Ion:276 Resp: 1561985

Ion Ratio Lower Upper

276 100

138 17.7 16.7 25.1

277 22.8 18.2 27.2

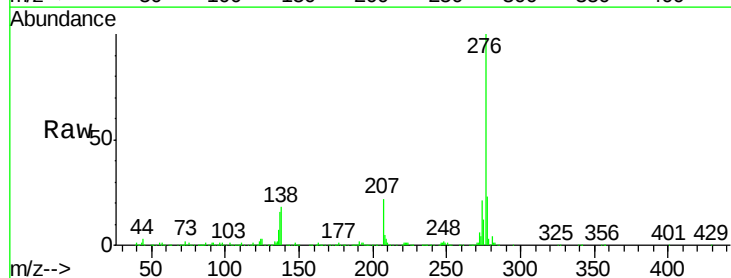

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

