

#15

N-Nitroso-di-n-propylamine

Concen: 1.741 ng/ul

RT: 8.29 min Scan# 902

Delta R.T. -0.10 min

Lab File: BN005418.D

Acq: 02 May 2019 16:43

Instrument :

BNA_N

ClientSampleId :

Tgt Ion: 70 Resp: 12794


Ion Ratio Lower Upper

70 100

42 396.2 53.8 80.8#

101 0.0 7.7 11.5#

130 0.0 15.0 22.4#



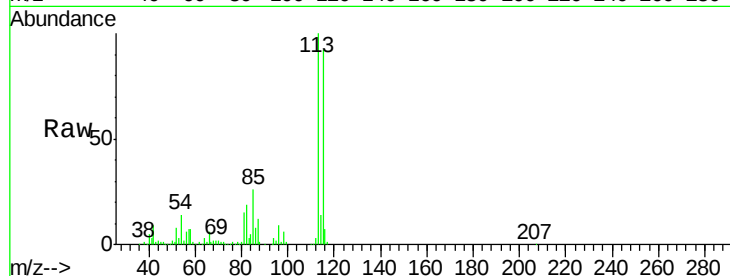


Abundance Ion 70.00 (69.70 to 70.70): BNC

Ion 42.00 (41.70 to 42.70): BNC

Ion 101.00 (100.70 to 101.70): BNC

Ion 130.00 (129.70 to 130.70): BNC

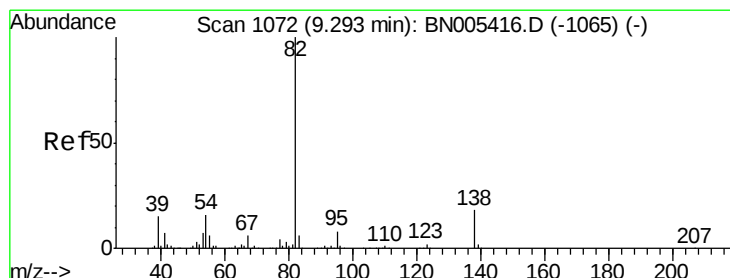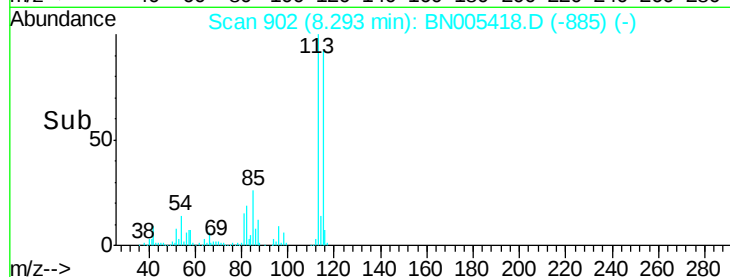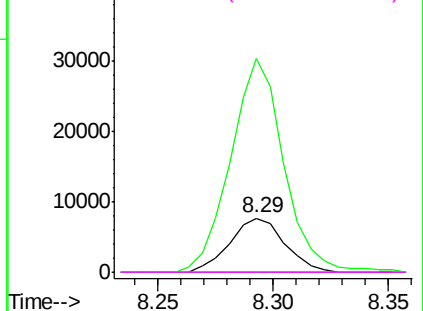

#21

Isophorone

Concen: 1.271 ng/ul

RT: 9.45 min Scan# 1098

Delta R.T. 0.15 min

Lab File: BN005418.D

Acq: 02 May 2019 16:43


Tgt Ion: 82 Resp: 26364

Ion Ratio Lower Upper

82 100

95 6.1 6.2 9.2#

138 0.0 13.2 19.8#

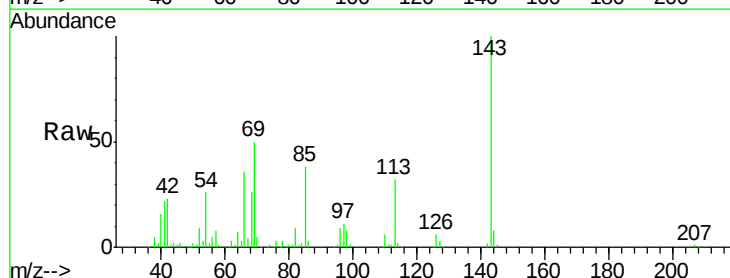

Abundance Ion 82.00 (81.70 to 82.70): BNC

Ion 95.00 (94.70 to 95.70): BNC

Ion 138.00 (137.70 to 138.70): BNC

