

#47

Acenaphthylene

Concen: 1.783 ng/ul

RT: 13.95 min Scan# 1863

Delta R.T. -0.00 min

Lab File: BN005419.D





Acq: 02 May 2019 17:18

Instrument :

BNA_N

ClientSampleId :

Tgt Ion:	152	Resp:	97507
Ion	Ratio	Lower	Upper
152	100		
151	20.5	15.8	23.8
153	13.7	9.8	14.8

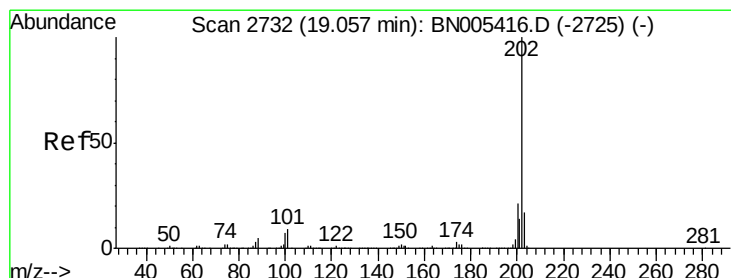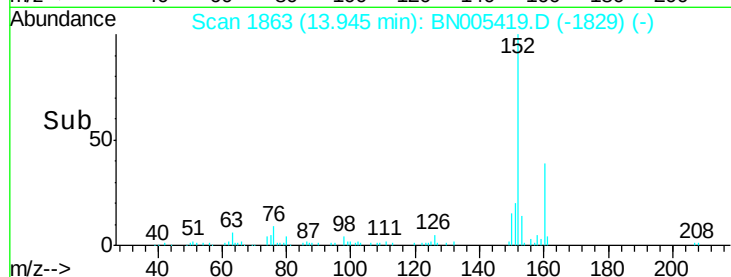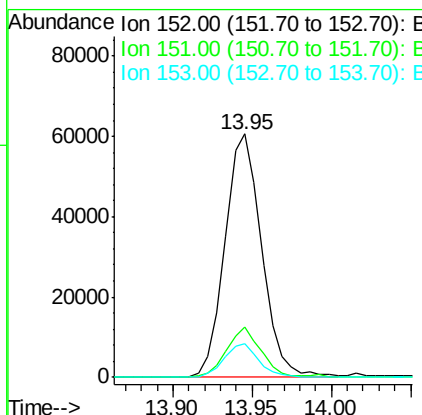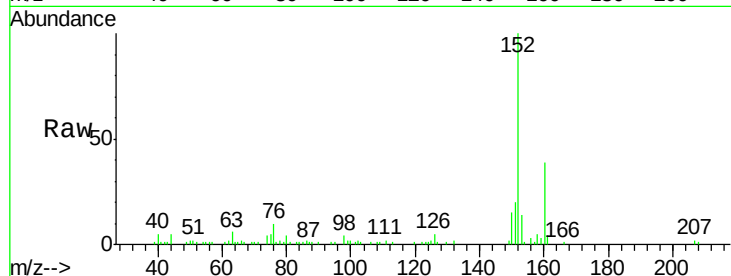

#76

Fluoranthene

Concen: 1.950 ng/ul

RT: 19.06 min Scan# 2732

Delta R.T. -0.00 min

Lab File: BN005419.D

Acq: 02 May 2019 17:18

Tgt Ion:	202	Resp:	146224
Ion	Ratio	Lower	Upper
202	100		
101	8.5	8.6	12.8#
100	6.0	6.3	9.5#

