

#84

Chrysene

Concen: 3.578 ng/ul

RT: 21.25 min Scan# 3105

Delta R.T. -0.00 min

Lab File: BN005419.D

Acq: 02 May 2019 17:18

Instrument :

BNA_N

ClientSampleId :


Tgt Ion:228 Resp: 256568

Ion Ratio Lower Upper

228 100

226 29.7 24.0 36.0




229 21.5 15.4 23.0

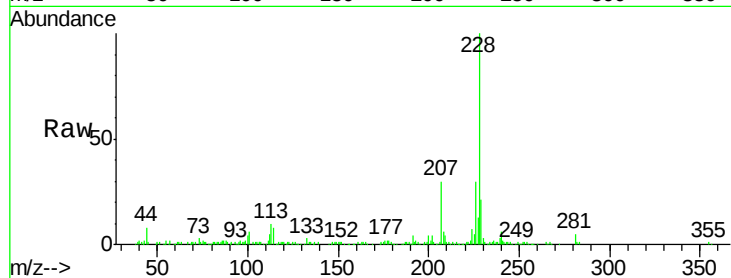

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

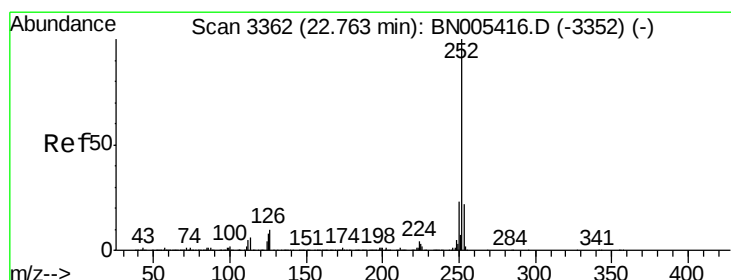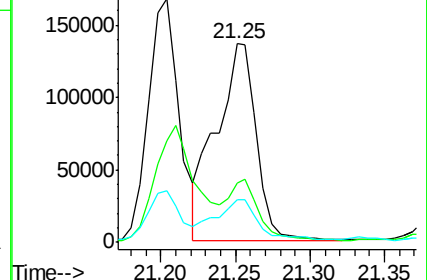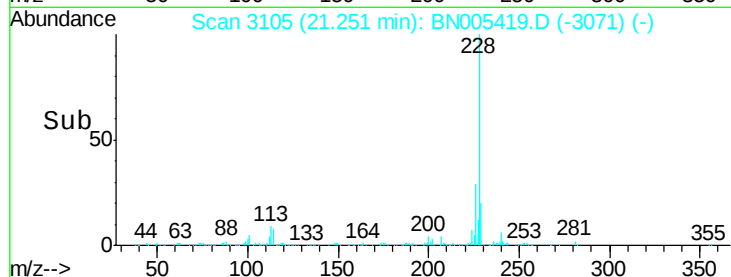

#87

Benzo(b)fluoranthene

Concen: 1.052 ng/ul

RT: 22.94 min Scan# 3393

Delta R.T. 0.18 min

Lab File: BN005419.D

Acq: 02 May 2019 17:18


Tgt Ion:252 Resp: 79877

Ion Ratio Lower Upper

252 100

253 22.0 17.7 26.5

125 9.6 8.4 12.6

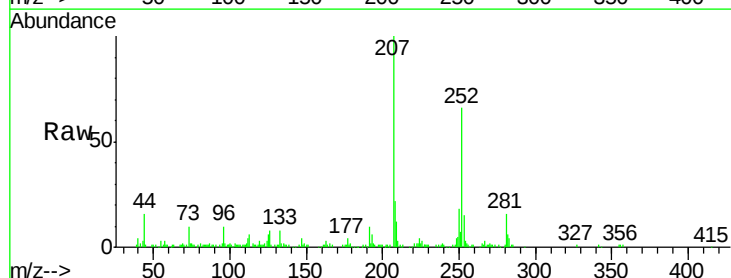

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

