

#88

Benzo(k)fluoranthene

Concen: 4.761 ng/ul

RT: 22.77 min Scan# 3364

Delta R.T. -0.03 min

Lab File: BN005419.D





Acq: 02 May 2019 17:18

Instrument :

BNA_N

ClientSampleId :

Tgt Ion:	252	Resp:	345343
Ion Ratio	Lower	Upper	
252	100		
253	22.1	17.4	26.0
125	7.9	7.5	11.3

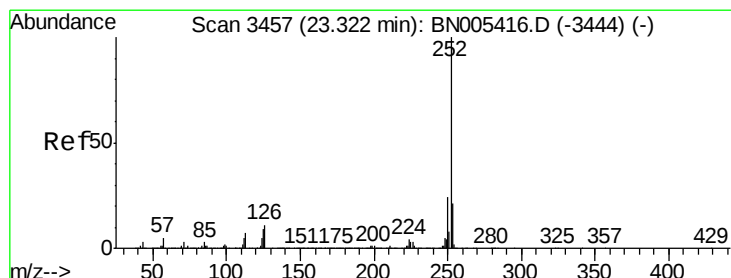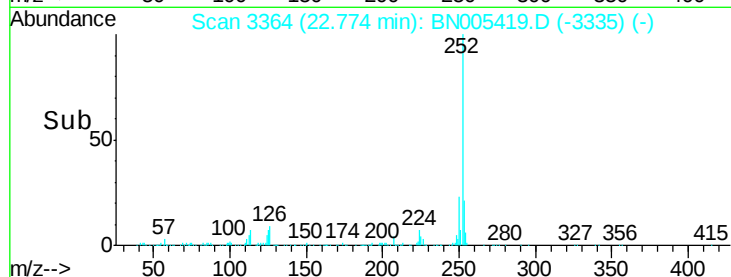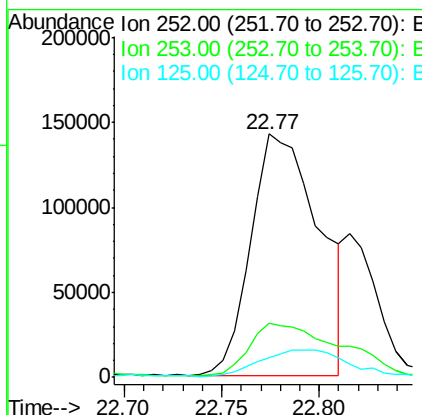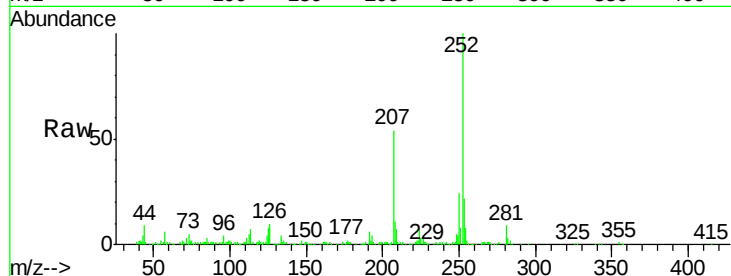

#90

Benzo(a)pyrene

Concen: 4.541 ng/ul

RT: 23.33 min Scan# 3459

Delta R.T. 0.01 min

Lab File: BN005419.D

Acq: 02 May 2019 17:18

Tgt Ion:	252	Resp:	324125
Ion Ratio	Lower	Upper	
252	100		
253	21.7	17.3	25.9
125	10.4	8.6	13.0

