

#6

Phenol

Concen: 26.870 ng/ul

RT: 6.80 min Scan# 649

Delta R.T. 0.01 min

Lab File: BN005420.D

Acq: 02 May 2019 17:53

Instrument :

BNA_N

ClientSampled :


Tgt Ion: 94 Resp: 514472

Ion Ratio Lower Upper

94 100

65 28.3 24.2 36.4




66 40.1 33.8 50.6

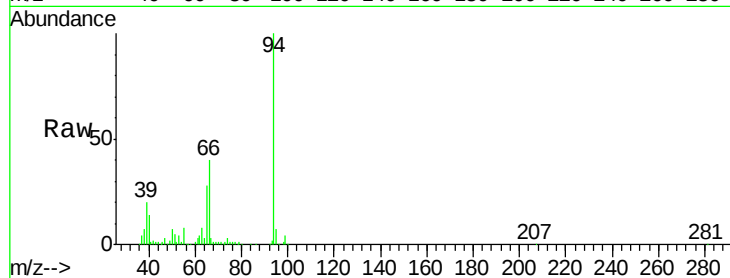

Abundance Ion 94.00 (93.70 to 94.70): BN005420.D (-614) (-)

Ion 65.00 (64.70 to 65.70): BN005420.D (-614) (-)

Ion 66.00 (65.70 to 66.70): BN005420.D (-614) (-)

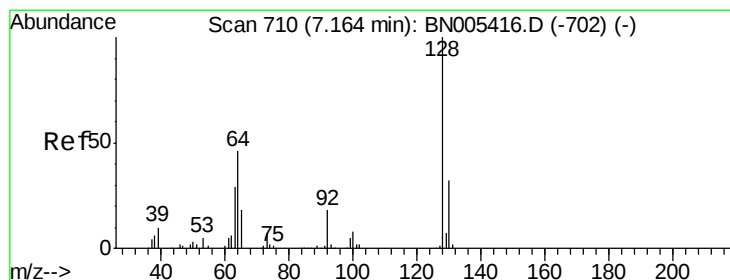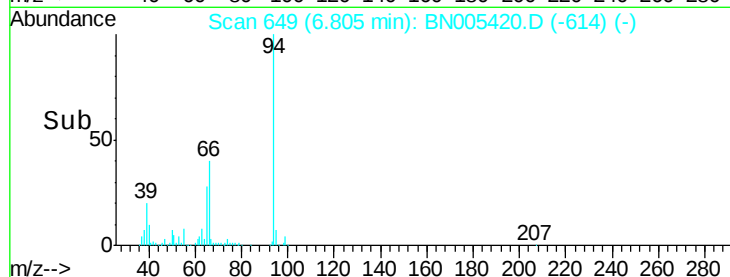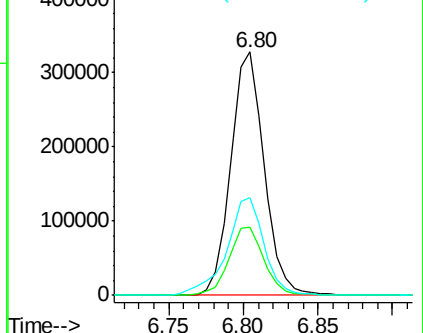

#10

2-Chlorophenol

Concen: 28.431 ng/ul

RT: 7.16 min Scan# 710

Delta R.T. -0.00 min

Lab File: BN005420.D

Acq: 02 May 2019 17:53


Tgt Ion: 128 Resp: 418725

Ion Ratio Lower Upper

128 100

64 46.6 42.3 63.5

130 33.1 26.5 39.7

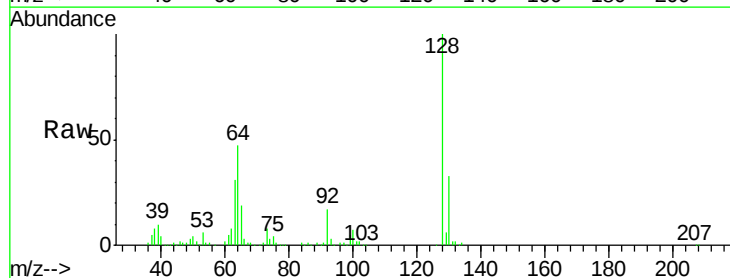

Abundance Ion 128.00 (127.70 to 128.70): BN005420.D (-676) (-)

Ion 64.00 (63.70 to 64.70): BN005420.D (-676) (-)

Ion 130.00 (129.70 to 130.70): BN005420.D (-676) (-)

