
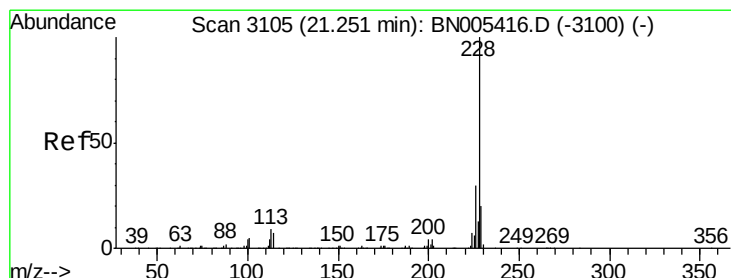
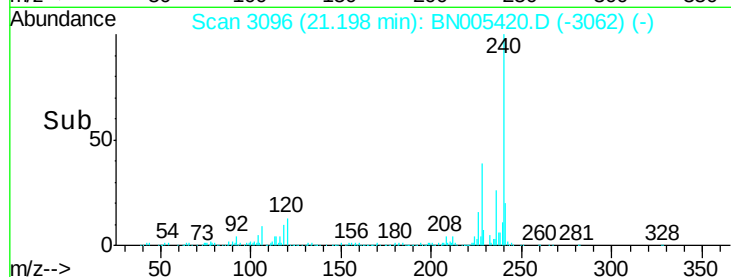
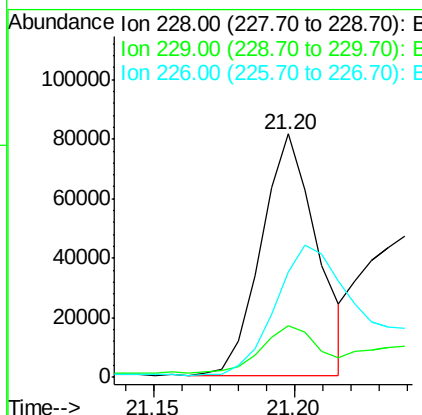


#82
Benzo(a)anthracene
Concen: 1.381 ng/ul
RT: 21.20 min Scan# 3096
Delta R.T. -0.00 min
Lab File: BN005420.D
Acq: 02 May 2019 17:53

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:228 Resp: 111456
Ion Ratio Lower Upper
228 100
229 21.2 15.8 23.6
226 43.1 21.4 32.2#

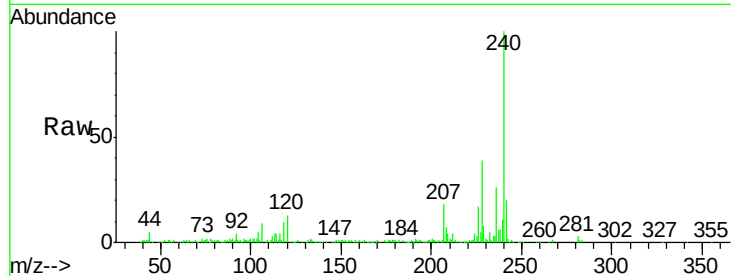

#84
Chrysene
Concen: 1.829 ng/ul
RT: 21.25 min Scan# 3105
Delta R.T. -0.00 min
Lab File: BN005420.D
Acq: 02 May 2019 17:53

Tgt Ion:228 Resp: 137032
Ion Ratio Lower Upper
228 100
226 33.3 24.0 36.0
229 23.1 15.4 23.0#

