
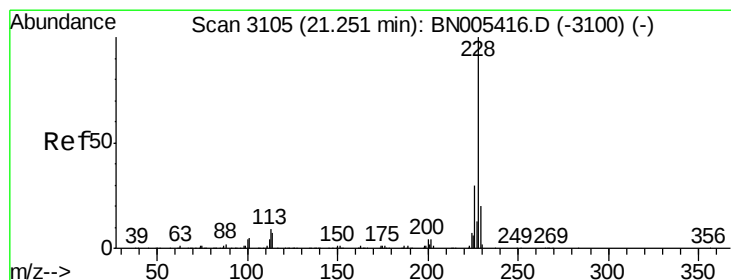
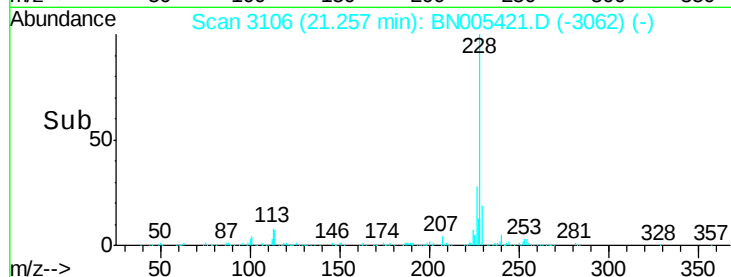
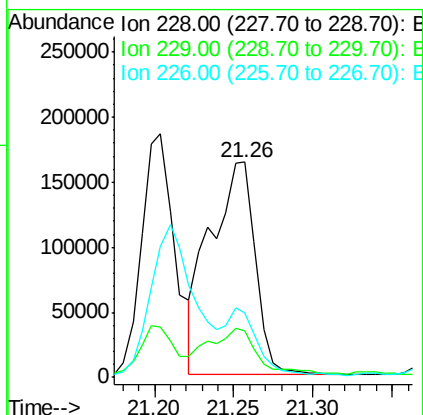


#82
Benzo(a)anthracene
Concen: 3.031 ng/ul
RT: 21.26 min Scan# 3106
Delta R.T. 0.06 min
Lab File: BN005421.D
Acq: 02 May 2019 18:27

Instrument :
BNA_N
ClientSampled :

Tgt Ion:228 Resp: 325470
Ion Ratio Lower Upper
228 100
229 21.7 15.8 23.6
226 29.7 21.4 32.2

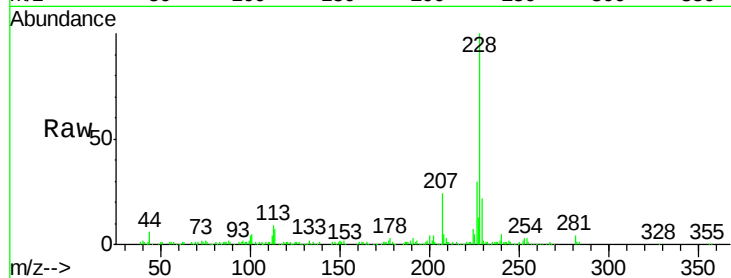

#84
Chrysene
Concen: 3.289 ng/ul
RT: 21.26 min Scan# 3106
Delta R.T. 0.01 min
Lab File: BN005421.D
Acq: 02 May 2019 18:27

Tgt Ion:228 Resp: 327797
Ion Ratio Lower Upper
228 100
226 29.7 24.0 36.0
229 21.7 15.4 23.0

