

#6

Phenol

Concen: 1.319 ng/ul

RT: 6.80 min Scan# 648

Delta R.T. 0.00 min

Lab File: BN005422.D

Acq: 02 May 2019 19:02

Instrument :

BNA_N

ClientSampleId :


Tgt Ion: 94 Resp: 29283

Ion Ratio Lower Upper

94 100

65 28.6 24.2 36.4




66 47.6 33.8 50.6

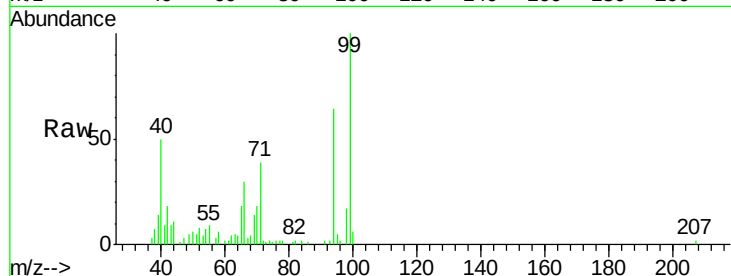

Abundance Ion 94.00 (93.70 to 94.70): BN005416.D (-642) (-)

Ion 65.00 (64.70 to 65.70): BN005416.D (-642) (-)

Ion 66.00 (65.70 to 66.70): BN005416.D (-642) (-)

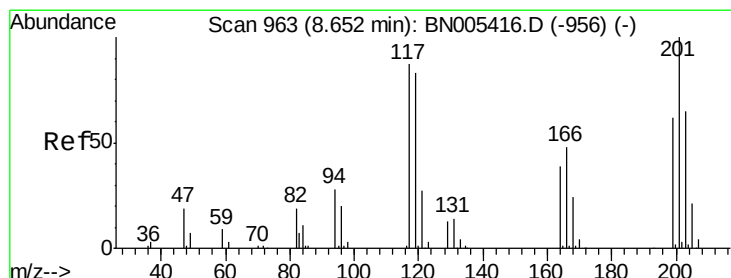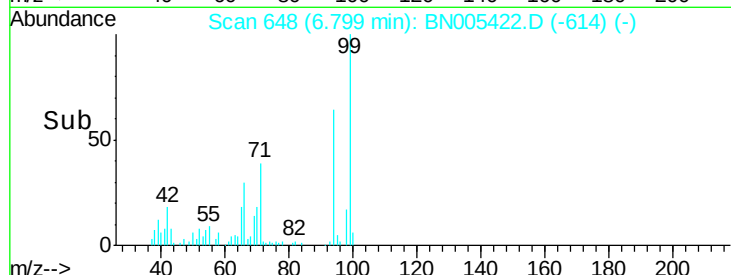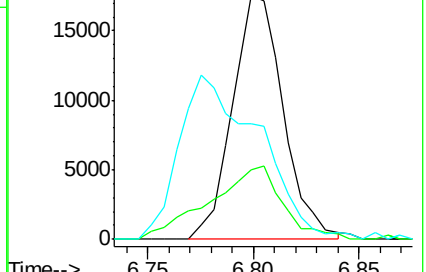

#17

Hexachloroethane

Concen: 2.260 ng/ul

RT: 8.68 min Scan# 968

Delta R.T. 0.03 min

Lab File: BN005422.D

Acq: 02 May 2019 19:02


Tgt Ion: 117 Resp: 16756

Ion Ratio Lower Upper

117 100

201 0.0 84.1 126.1#

199 0.0 51.2 76.8#

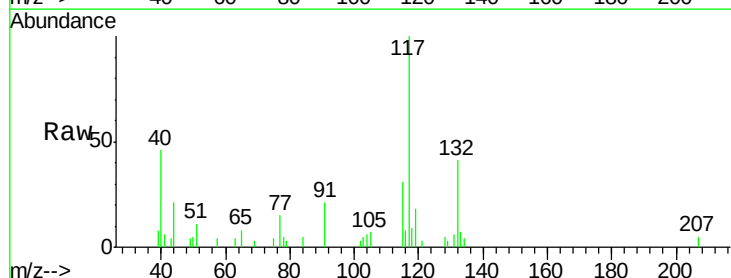

Abundance Ion 117.00 (116.70 to 117.70): BN005416.D (-956) (-)

Ion 201.00 (200.70 to 201.70): BN005416.D (-956) (-)

Ion 199.00 (198.70 to 199.70): BN005416.D (-956) (-)

