

#28

Naphthalene

Concen: 5.533 ng/ul

RT: 10.40 min Scan# 1260

Delta R.T. 0.00 min

Lab File: BN005422.D

Acq: 02 May 2019 19:02

Instrument :

BNA_N

ClientSampleId :


Tgt Ion:128 Resp: 311035

Ion Ratio Lower Upper

128 100

129 10.5 9.2 13.8




127 13.4 10.7 16.1

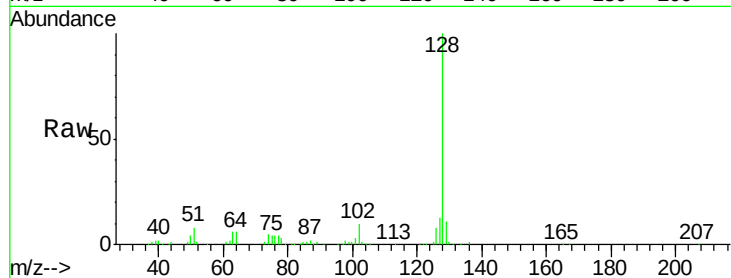

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

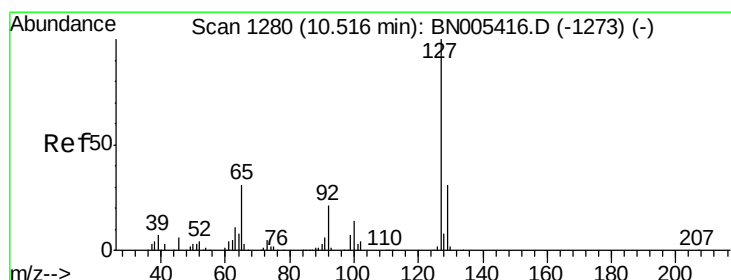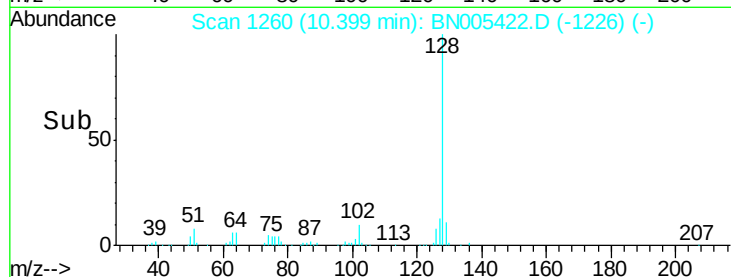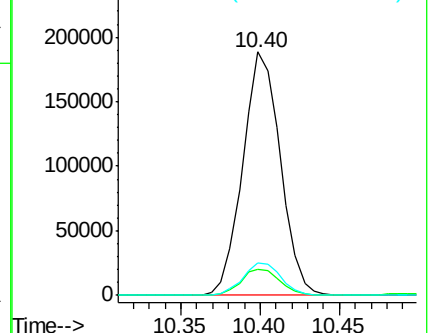

#30

4-Chloroaniline

Concen: 2.344 ng/ul

RT: 10.40 min Scan# 1260

Delta R.T. -0.12 min

Lab File: BN005422.D


Acq: 02 May 2019 19:02

Tgt Ion:127 Resp: 42581

Ion Ratio Lower Upper

127 100

129 78.4 25.8 38.6#

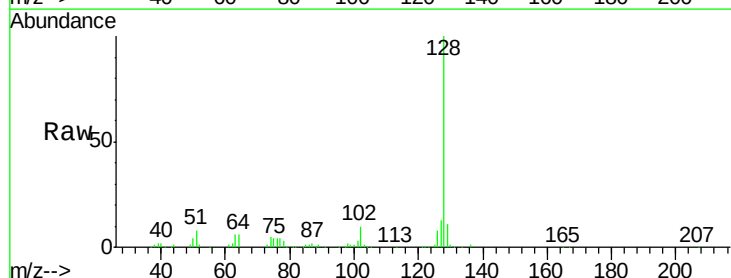

Abundance Ion 127.00 (126.70 to 127.70): E

Ion 129.00 (128.70 to 129.70): E

