
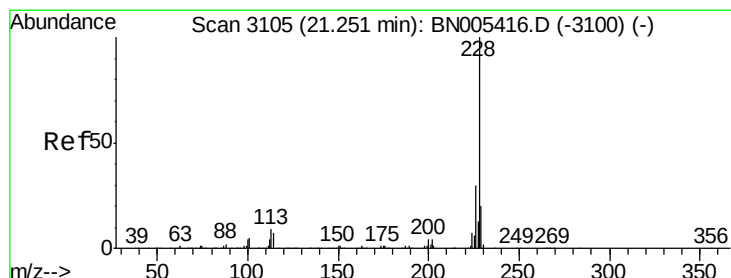
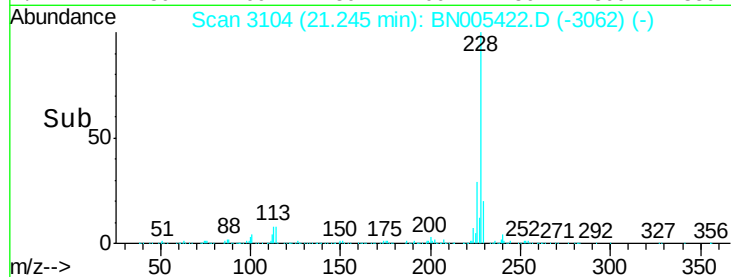
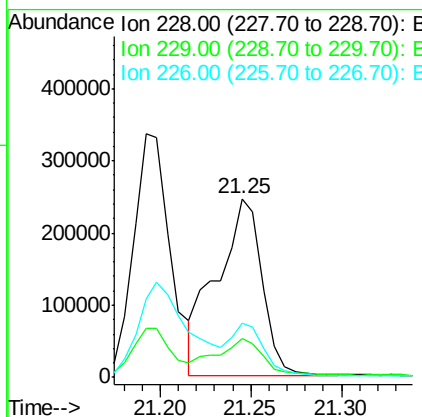


#82  
Benzo(a)anthracene  
Concen: 4.017 ng/ul  
RT: 21.25 min Scan# 3104  
Delta R.T. 0.05 min  
Lab File: BN005422.D  
Acq: 02 May 2019 19:02

Instrument :  
BNA\_N  
ClientSampleId :

Tgt Ion:228 Resp: 431625  
Ion Ratio Lower Upper  
228 100  
229 22.0 15.8 23.6  
226 30.2 21.4 32.2

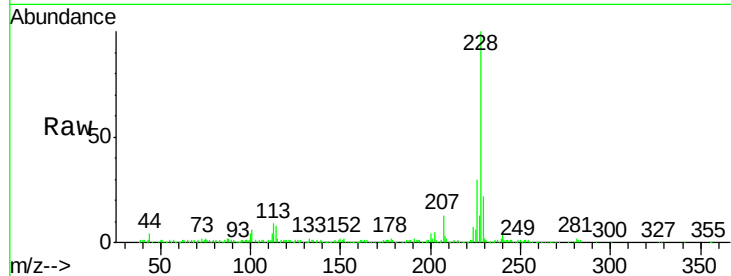

#84  
Chrysene  
Concen: 4.261 ng/ul  
RT: 21.25 min Scan# 3104  
Delta R.T. -0.01 min  
Lab File: BN005422.D  
Acq: 02 May 2019 19:02

Tgt Ion:228 Resp: 424890  
Ion Ratio Lower Upper  
228 100  
226 30.2 24.0 36.0  
229 22.0 15.4 23.0

