

#6

Phenol

Concen: 1.398 ng/ul

RT: 6.80 min Scan# 649

Delta R.T. 0.01 min

Lab File: BN005424.D

Acq: 02 May 2019 20:11

Instrument :

BNA_N

ClientSampled :


Tgt Ion: 94 Resp: 29714

Ion Ratio Lower Upper




94 100

65 34.2 24.2 36.4

66 46.6 33.8 50.6

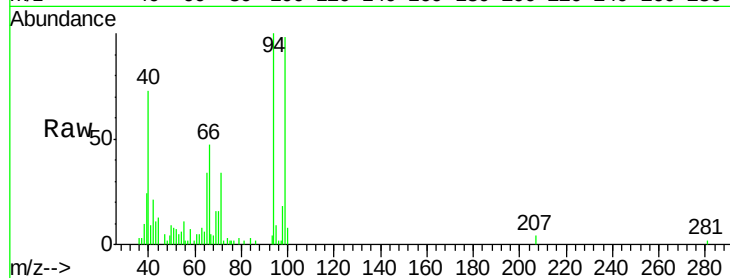

Abundance Ion 94.00 (93.70 to 94.70): BNC
Ion 65.00 (64.70 to 65.70): BNC
Ion 66.00 (65.70 to 66.70): BNC

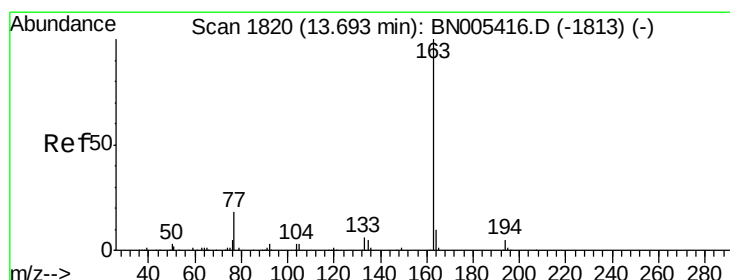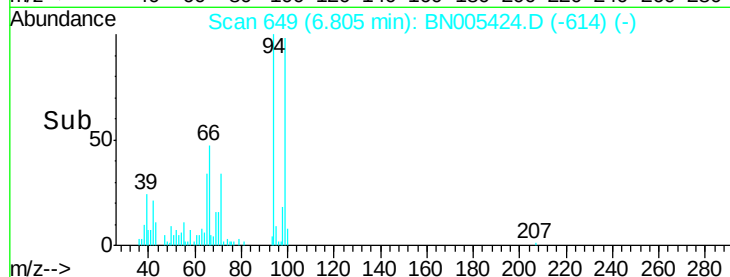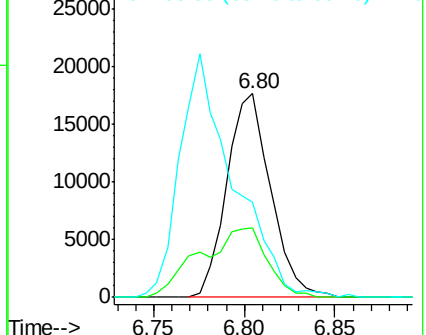

#44

Dimethylphthalate

Concen: 10.832 ng/ul

RT: 13.69 min Scan# 1820

Delta R.T. -0.00 min

Lab File: BN005424.D

Acq: 02 May 2019 20:11


Tgt Ion: 163 Resp: 604607

Ion Ratio Lower Upper

163 100

194 4.6 3.4 5.0

164 10.1 8.1 12.1

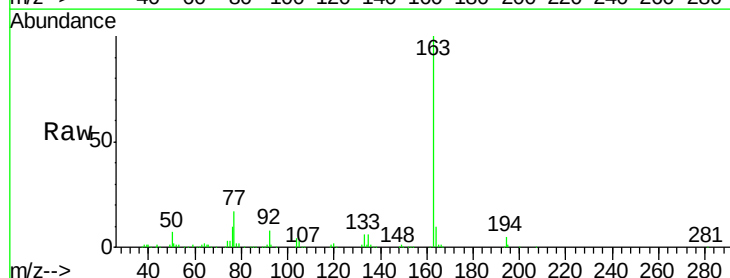

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

