

#6

Phenol

Concen: 1.679 ng/ul

RT: 6.80 min Scan# 648

Delta R.T. -0.00 min

Lab File: BN005425.D

Acq: 02 May 2019 20:45

Instrument :

BNA\_N

ClientSampleId :


Tgt Ion: 94 Resp: 35185

Ion Ratio Lower Upper

94 100

65 30.6 24.2 36.4




66 52.7 33.8 50.6#

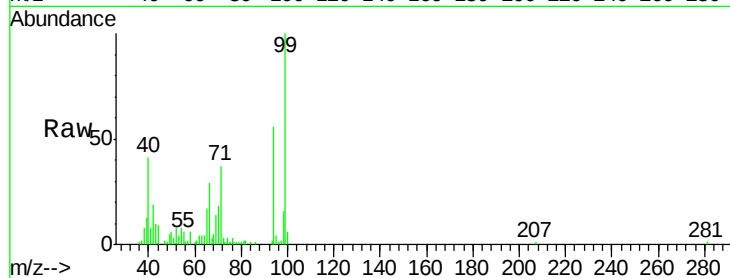

Abundance Ion 94.00 (93.70 to 94.70): BN005416.D (-642) (-)

Ion 65.00 (64.70 to 65.70): BN005416.D (-642) (-)

Ion 66.00 (65.70 to 66.70): BN005416.D (-642) (-)

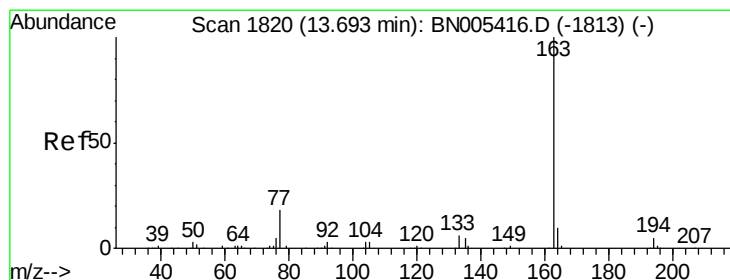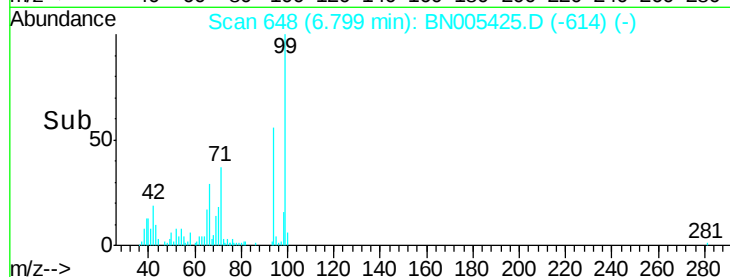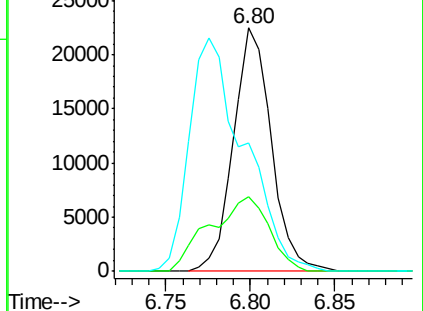

#44

Dimethylphthalate

Concen: 14.754 ng/ul

RT: 13.69 min Scan# 1820

Delta R.T. -0.00 min

Lab File: BN005425.D

Acq: 02 May 2019 20:45


Tgt Ion: 163 Resp: 770318

Ion Ratio Lower Upper

163 100

194 4.7 3.4 5.0

164 9.8 8.1 12.1

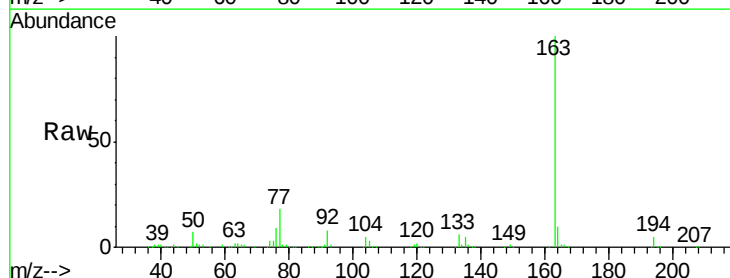

Abundance Ion 163.00 (162.70 to 163.70): BN005416.D (-1813) (-)

Ion 194.00 (193.70 to 194.70): BN005416.D (-1813) (-)

Ion 164.00 (163.70 to 164.70): BN005416.D (-1813) (-)

