
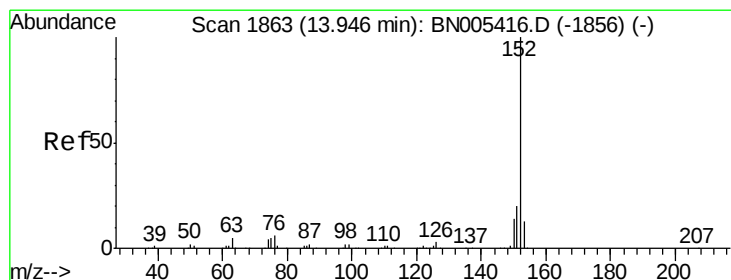
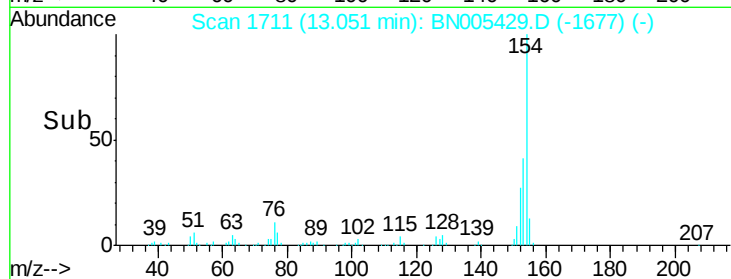
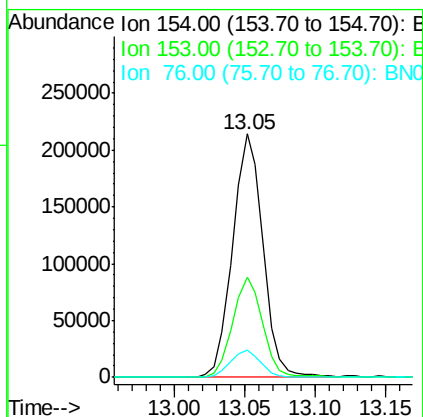


#40
 1,1'-Biphenyl
 Concen: 5.406 ng/ul
 RT: 13.05 min Scan# 1711
 Delta R.T. -0.00 min
 Lab File: BN005429.D
 Acq: 02 May 2019 23:03

Instrument :
 BNA_N
 ClientSampled :

Tgt Ion	Ratio	Lower	Upper
154	100		
153	41.2	32.6	49.0
76	11.3	10.4	15.6

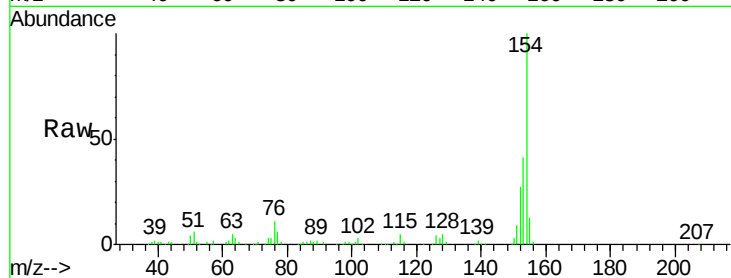

#47
 Acenaphthylene
 Concen: 14.264 ng/ul
 RT: 13.95 min Scan# 1863
 Delta R.T. -0.00 min
 Lab File: BN005429.D
 Acq: 02 May 2019 23:03

Tgt Ion	Ratio	Lower	Upper
152	100		
151	19.1	15.8	23.8
153	13.6	9.8	14.8

