





#71
 Anthracene
 Concen: 51.498 ng/ul
 RT: 17.11 min Scan# 2401
 Delta R.T. -0.01 min
 Lab File: BN005429.D
 Acq: 02 May 2019 23:03

Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion:178 Resp: 813339
 Ion Ratio Lower Upper
 178 100
 179 15.8 12.3 18.5
 176 17.9 15.1 22.7

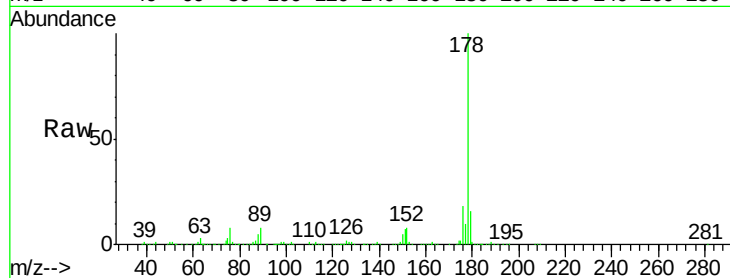


Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 179.00 (178.70 to 179.70): E
 Ion 176.00 (175.70 to 176.70): E

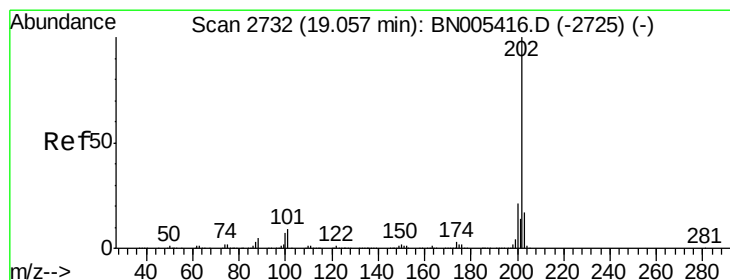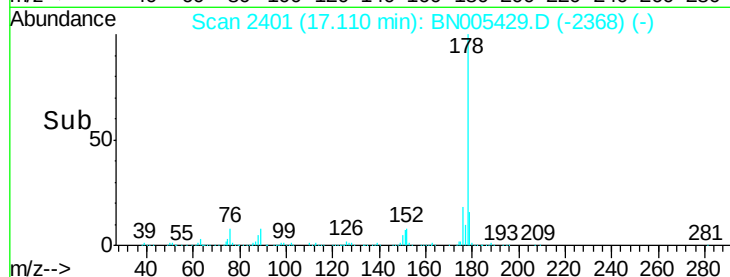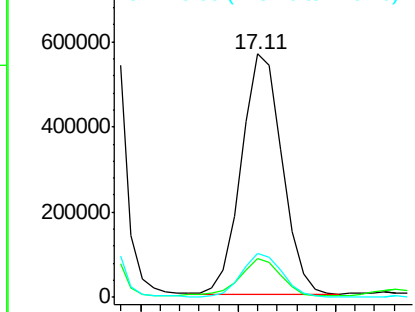

#76
 Fluoranthene
 Concen: 27.928 ng/ul
 RT: 19.20 min Scan# 2757
 Delta R.T. 0.15 min
 Lab File: BN005429.D
 Acq: 02 May 2019 23:03

Tgt Ion:202 Resp: 480272
 Ion Ratio Lower Upper
 202 100
 101 8.7 8.6 12.8
 100 6.7 6.3 9.5

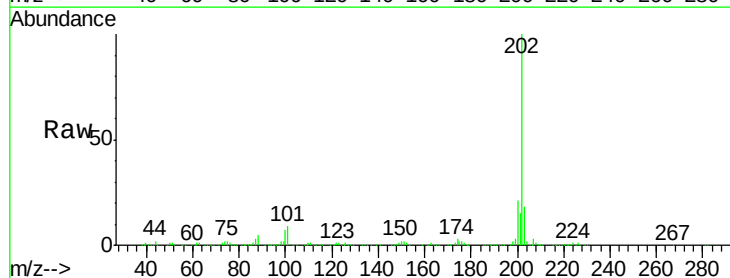

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

