





#81
 3,3'-Dichlorobenzidine
 Concen: 4.351 ng/ul
 RT: 21.20 min Scan# 3096
 Delta R.T. 0.06 min
 Lab File: BN005429.D
 Acq: 02 May 2019 23:03

Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion:252 Resp: 207
 Ion Ratio Lower Upper
 252 100
 254 0.0 51.1 76.7#
 126 594.7 9.4 14.0#

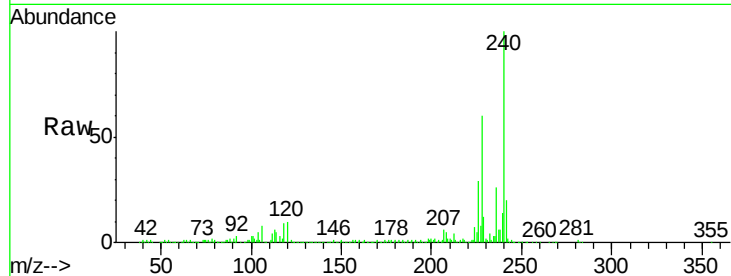


Abundance Ion 252.00 (251.70 to 252.70): E
 Ion 254.00 (253.70 to 254.70): E
 Ion 126.00 (125.70 to 126.70): E

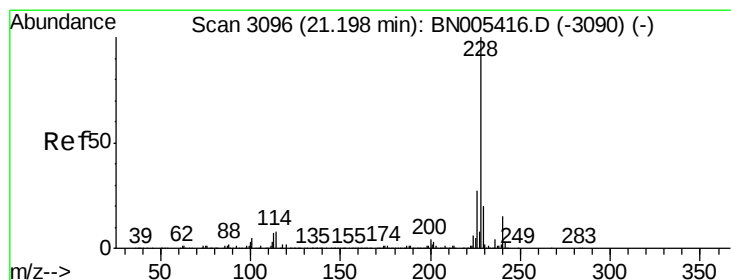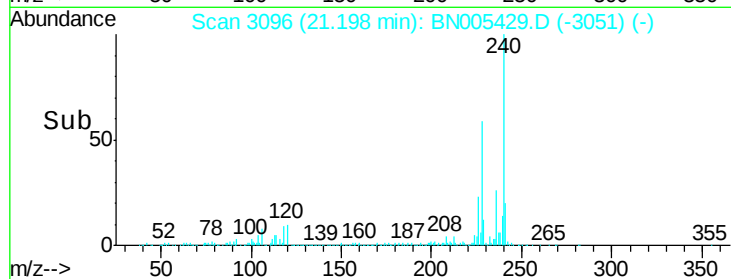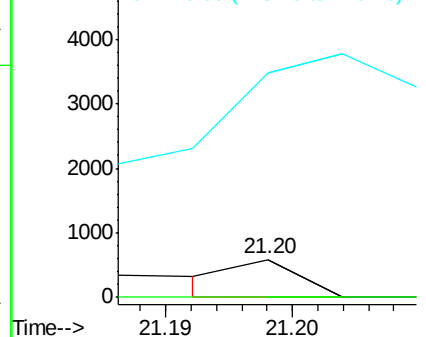

#82
 Benzo(a)anthracene
 Concen: 4279.351 ng/ul
 RT: 21.25 min Scan# 3104
 Delta R.T. 0.05 min
 Lab File: BN005429.D
 Acq: 02 May 2019 23:03

Tgt Ion:228 Resp: 633869
 Ion Ratio Lower Upper
 228 100
 229 20.6 15.8 23.6
 226 30.0 21.4 32.2

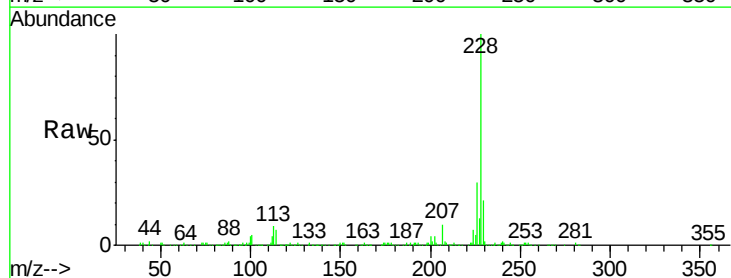

Abundance Ion 228.00 (227.70 to 228.70): E
 Ion 229.00 (228.70 to 229.70): E
 Ion 226.00 (225.70 to 226.70): E

