
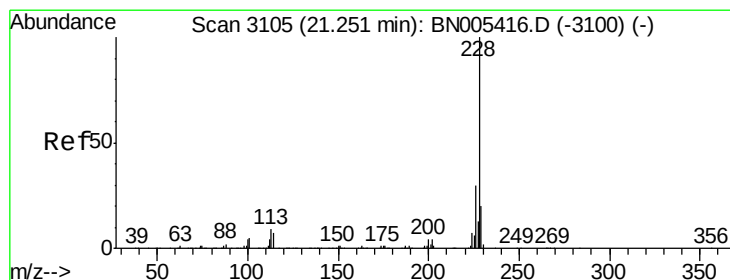
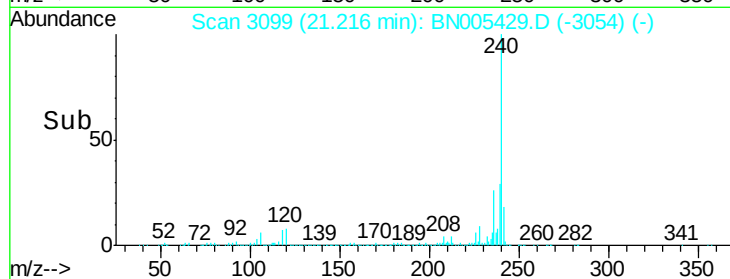
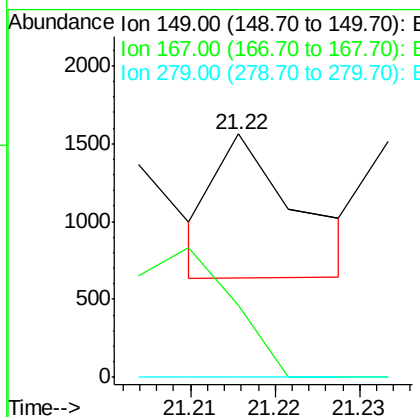


#83
 Bis(2-ethylhexyl)phthalate
 Concen: 6.591 ng/ul
 RT: 21.22 min Scan# 3099
 Delta R.T. 0.06 min
 Lab File: BN005429.D
 Acq: 02 May 2019 23:03

Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion:149 Resp: 616
 Ion Ratio Lower Upper
 149 100
 167 29.5 22.3 33.5
 279 0.0 3.3 4.9#

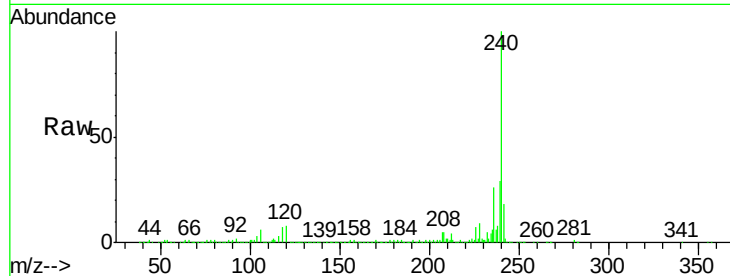

#84
 Chrysene
 Concen: 4602.534 ng/ul
 RT: 21.25 min Scan# 3104
 Delta R.T. -0.01 min
 Lab File: BN005429.D
 Acq: 02 May 2019 23:03

Tgt Ion:228 Resp: 632718
 Ion Ratio Lower Upper
 228 100
 226 30.0 24.0 36.0
 229 20.6 15.4 23.0

