
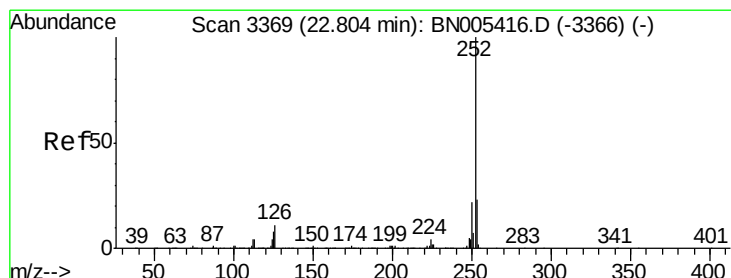
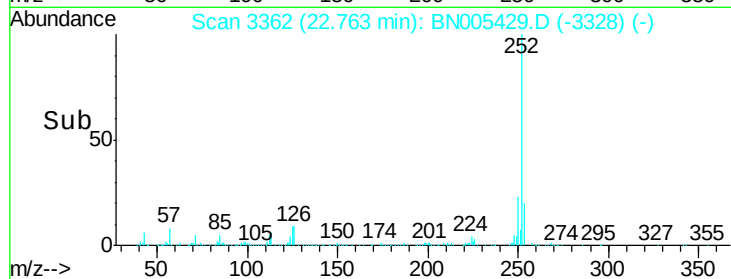
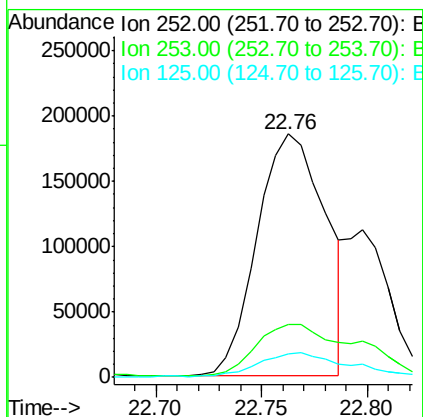


#87
 Benzo(b)fluoranthene
 Concen: 4.270 ng/ul
 RT: 22.76 min Scan# 3362
 Delta R.T. -0.00 min
 Lab File: BN005429.D
 Acq: 02 May 2019 23:03

Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion:252 Resp: 417018
 Ion Ratio Lower Upper
 252 100
 253 21.6 17.7 26.5
 125 9.4 8.4 12.6

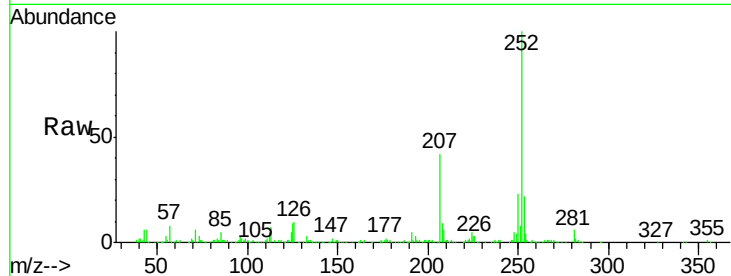

#88
 Benzo(k)fluoranthene
 Concen: 4.471 ng/ul
 RT: 22.76 min Scan# 3362
 Delta R.T. -0.04 min
 Lab File: BN005429.D
 Acq: 02 May 2019 23:03

Tgt Ion:252 Resp: 417018
 Ion Ratio Lower Upper
 252 100
 253 21.6 17.4 26.0
 125 9.4 7.5 11.3

