

#47

Acenaphthylene

Concen: 4.362 ng/ul

RT: 13.95 min Scan# 1863

Delta R.T. -0.00 min

Lab File: BN005430.D

Acq: 02 May 2019 23:38

Instrument :

BNA_N

ClientSampled :


Tgt Ion:152 Resp: 273210

Ion Ratio Lower Upper

152 100

151 20.7 15.8 23.8




153 14.5 9.8 14.8

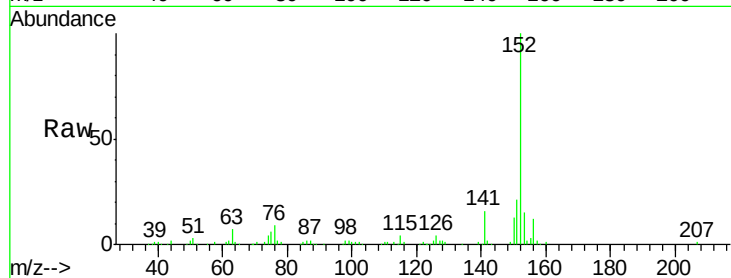

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

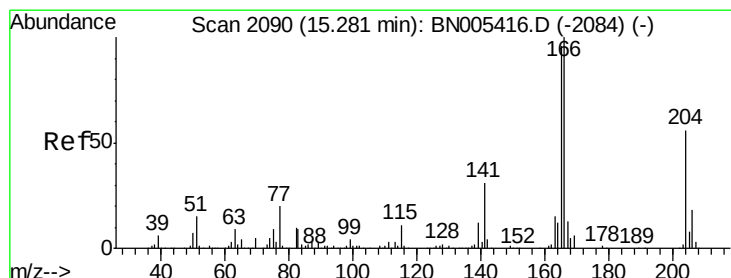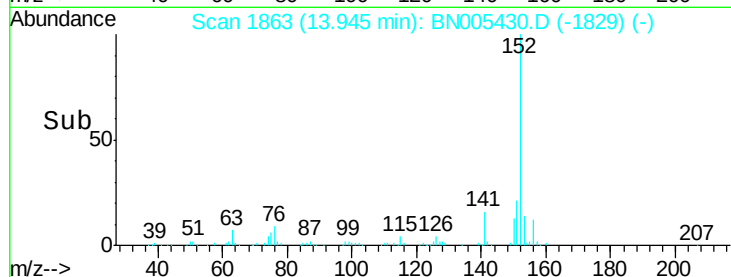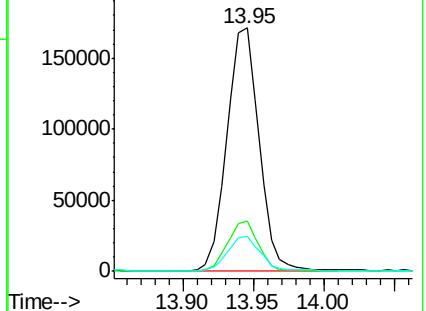

#58

Fluorene

Concen: 4.135 ng/ul

RT: 15.28 min Scan# 2090

Delta R.T. -0.00 min

Lab File: BN005430.D

Acq: 02 May 2019 23:38


Tgt Ion:166 Resp: 198620

Ion Ratio Lower Upper

166 100

165 94.4 80.0 120.0

167 13.8 10.7 16.1

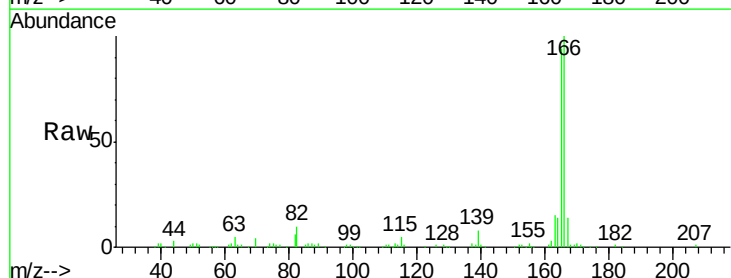

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

