
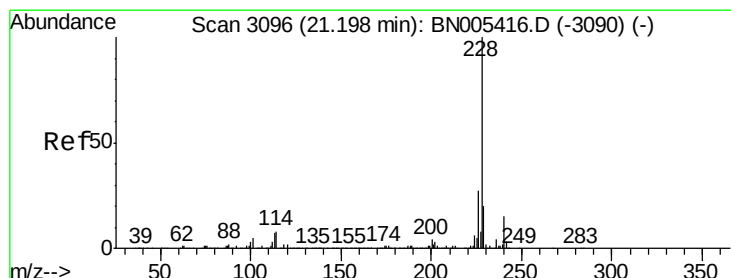
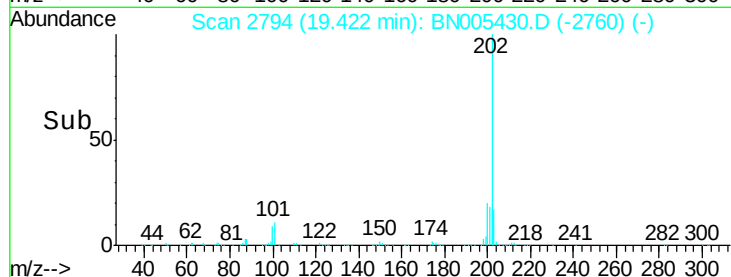
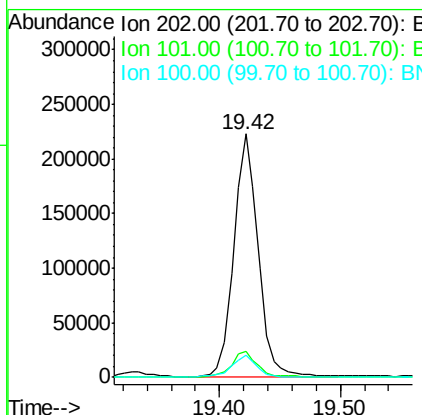


#79
 Pyrene
 Concen: 3.129 ng/ul
 RT: 19.42 min Scan# 2794
 Delta R.T. -0.00 min
 Lab File: BN005430.D
 Acq: 02 May 2019 23:38

Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion	Ratio	Lower	Upper
202	100		
101	10.7	10.3	15.5
100	8.9	7.9	11.9

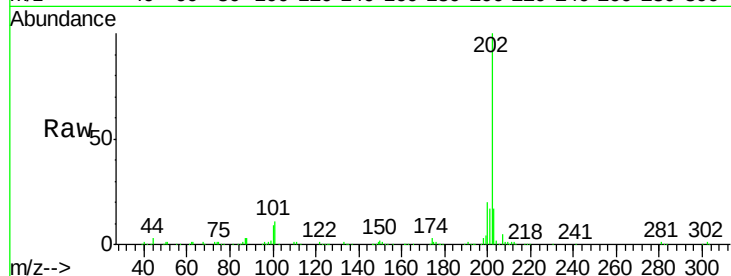

#82
 Benzo(a)anthracene
 Concen: 1.144 ng/ul
 RT: 21.20 min Scan# 3096
 Delta R.T. -0.00 min
 Lab File: BN005430.D
 Acq: 02 May 2019 23:38

Tgt Ion	Ratio	Lower	Upper
228	100		
229	21.4	15.8	23.6
226	31.4	21.4	32.2

