

#2

1,4-Dioxane

Concen: 7.327 ng/uL

RT: 3.25 min Scan# 44

Delta R.T. -0.00 min

Lab File: BN005431.D

Acq: 03 May 2019 00:12

Instrument :

BNA_N

ClientSampleId :


Tgt Ion: 88 Resp: 46376

Ion Ratio Lower Upper

88 100

43 32.4 25.3 37.9




58 79.9 62.3 93.5

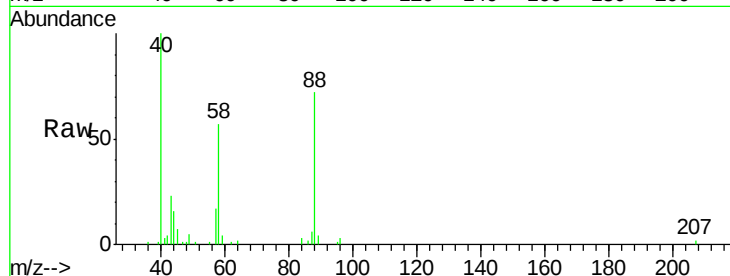

Abundance Ion 88.00 (87.70 to 88.70): BN005431.D (-10) (-)

Ion 43.00 (42.70 to 43.70): BN005431.D (-10) (-)

Ion 58.00 (57.70 to 58.70): BN005431.D (-10) (-)

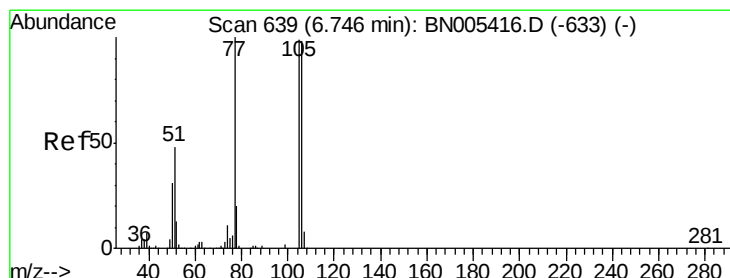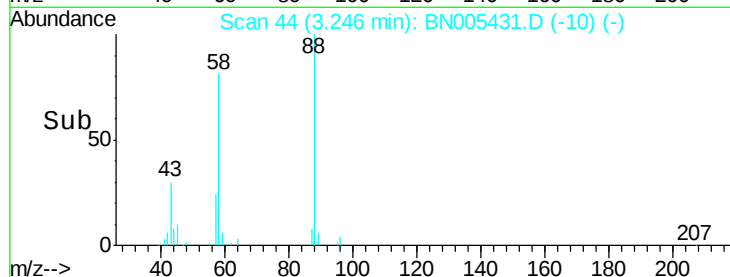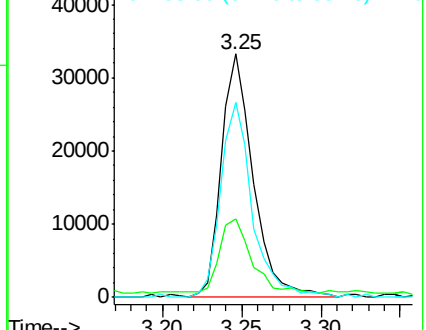

#4

Benzaldehyde

Concen: 18.933 ng/uL

RT: 6.75 min Scan# 639

Delta R.T. -0.00 min

Lab File: BN005431.D

Acq: 03 May 2019 00:12


Tgt Ion: 77 Resp: 299390

Ion Ratio Lower Upper

77 100

105 103.7 77.4 116.2

106 98.0 76.3 114.5

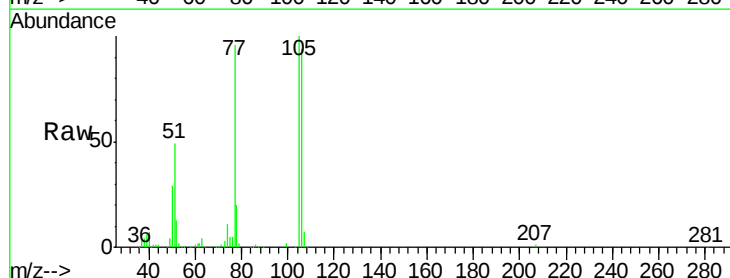

Abundance Ion 77.00 (76.70 to 77.70): BN005431.D (-605) (-)

Ion 105.00 (104.70 to 105.70): BN005431.D (-605) (-)

Ion 106.00 (105.70 to 106.70): BN005431.D (-605) (-)

