

#10

2-Chlorophenol

Concen: 20.396 ng/ul

RT: 7.16 min Scan# 710

Delta R.T. -0.00 min

Lab File: BN005431.D

Acq: 03 May 2019 00:12

Instrument :

BNA_N

ClientSampleId :


Tgt Ion:128 Resp: 360090

Ion Ratio Lower Upper

128 100

64 48.3 42.3 63.5




130 33.0 26.5 39.7

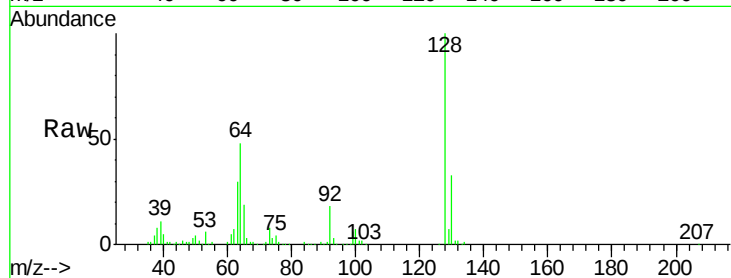

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 64.00 (63.70 to 64.70): BNO

Ion 130.00 (129.70 to 130.70): E

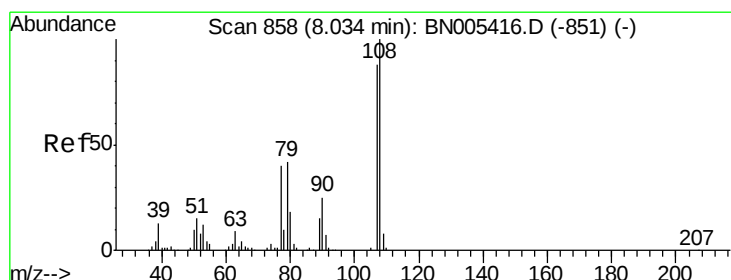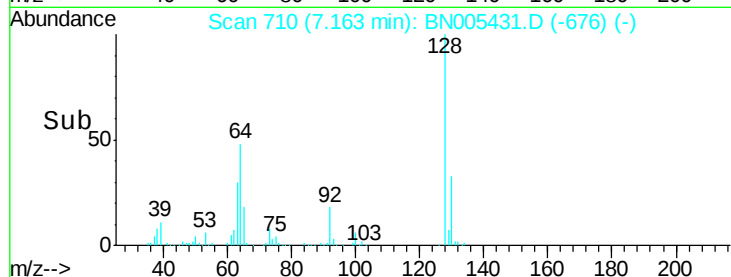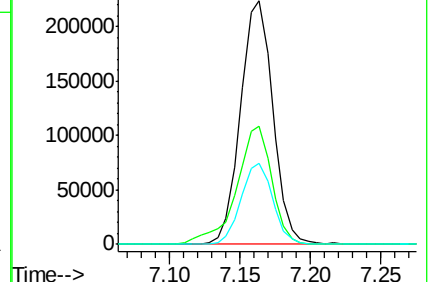

#11

2-Methylphenol

Concen: 20.628 ng/ul

RT: 8.03 min Scan# 857

Delta R.T. -0.01 min

Lab File: BN005431.D


Acq: 03 May 2019 00:12

Tgt Ion:108 Resp: 354780

Ion Ratio Lower Upper

108 100

107 89.5 72.9 109.3

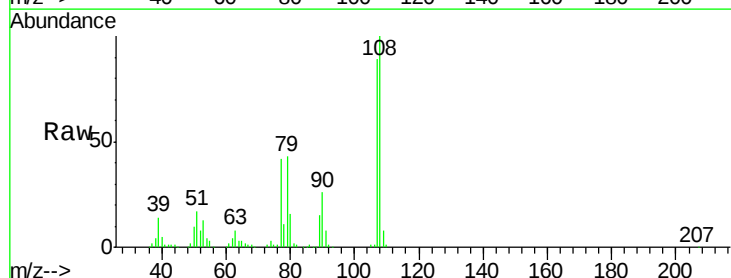

Abundance Ion 108.00 (107.70 to 108.70): E

Ion 107.00 (106.70 to 107.70): E

