





#17
Hexachloroethane
Concen: 19.679 ng/ul
RT: 8.65 min Scan# 963
Delta R.T. -0.00 min
Lab File: BN005431.D
Acq: 03 May 2019 00:12

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:117 Resp: 150870
Ion Ratio Lower Upper
117 100
201 110.2 84.1 126.1
199 70.5 51.2 76.8

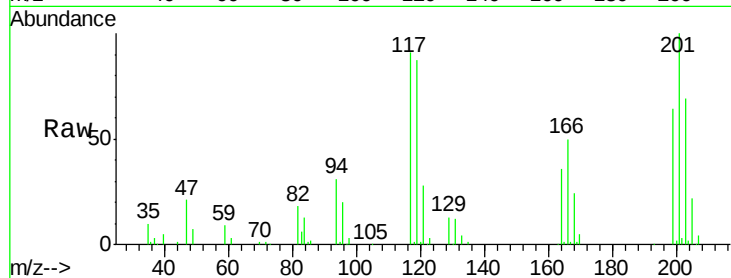


Abundance Ion 117.00 (116.70 to 117.70): E
Ion 201.00 (200.70 to 201.70): E
Ion 199.00 (198.70 to 199.70): E

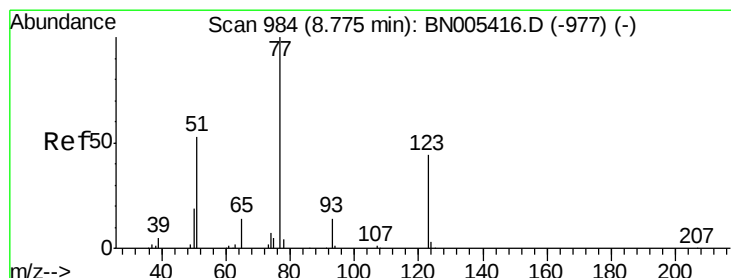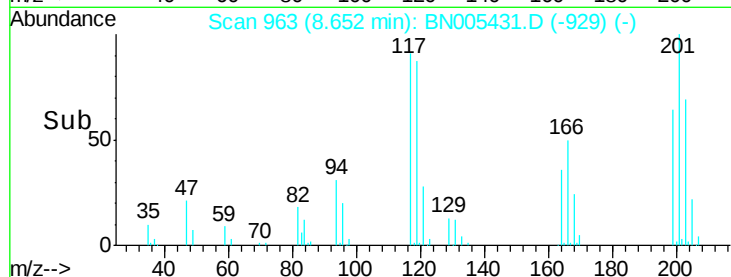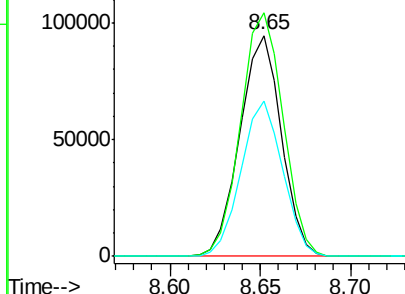

#20
Nitrobenzene
Concen: 19.470 ng/ul
RT: 8.78 min Scan# 984
Delta R.T. -0.00 min
Lab File: BN005431.D
Acq: 03 May 2019 00:12

Tgt Ion: 77 Resp: 425038
Ion Ratio Lower Upper
77 100
123 49.3 32.6 49.0#
65 14.8 11.6 17.4

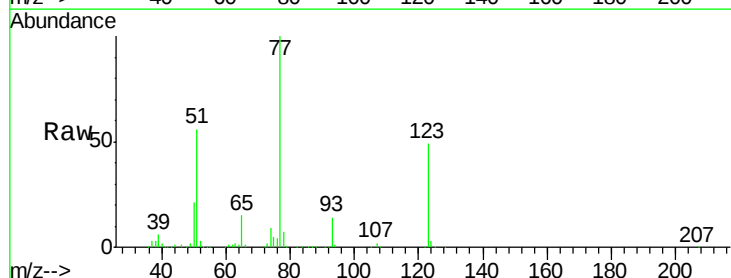

Abundance Ion 77.00 (76.70 to 77.70): BNC
Ion 123.00 (122.70 to 123.70): E
Ion 65.00 (64.70 to 65.70): BNC

