

#24

2,4-Dimethylphenol

Concen: 20.214 ng/ul

RT: 9.55 min Scan# 1115

Delta R.T. -0.00 min

Lab File: BN005431.D

Acq: 03 May 2019 00:12

Instrument :

BNA_N

ClientSampleId :


Tgt Ion: 107 Resp: 461211

Ion Ratio Lower Upper

107 100

121 50.3 37.8 56.8




122 79.2 65.0 97.4

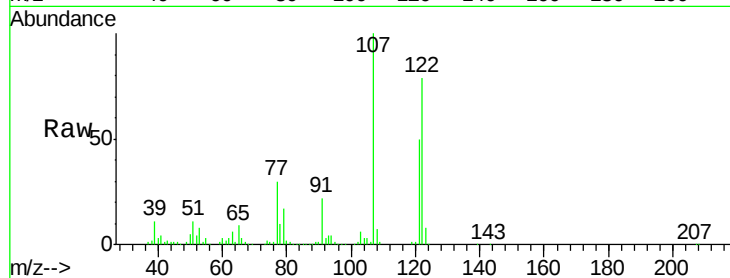

Abundance Ion 107.00 (106.70 to 107.70): E

Ion 121.00 (120.70 to 121.70): E

Ion 122.00 (121.70 to 122.70): E

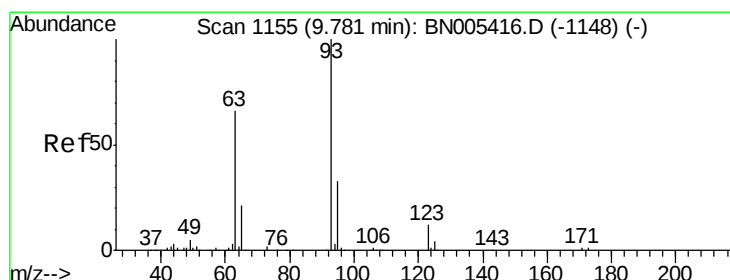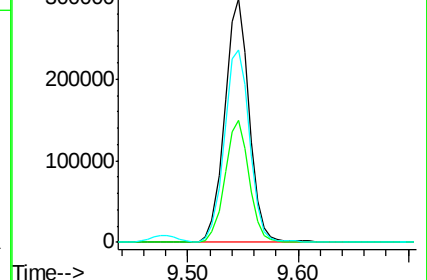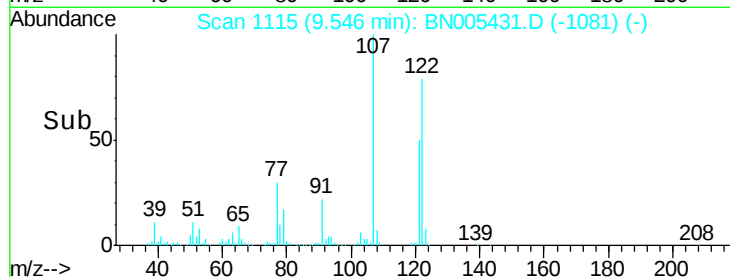

#25

Bis(2-Chloroethoxy)methane

Concen: 19.231 ng/ul

RT: 9.78 min Scan# 1155

Delta R.T. -0.00 min

Lab File: BN005431.D

Acq: 03 May 2019 00:12


Tgt Ion: 93 Resp: 522362

Ion Ratio Lower Upper

93 100

95 32.0 26.6 39.8

123 11.3 8.9 13.3

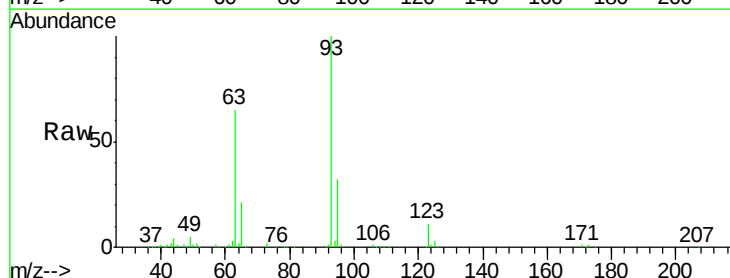

Abundance Ion 93.00 (92.70 to 93.70): BNC

Ion 95.00 (94.70 to 95.70): BNC

Ion 123.00 (122.70 to 123.70): E

