
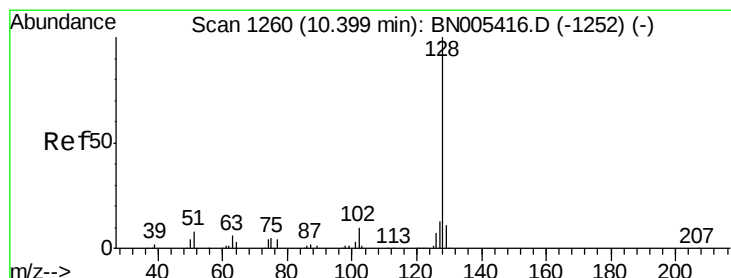
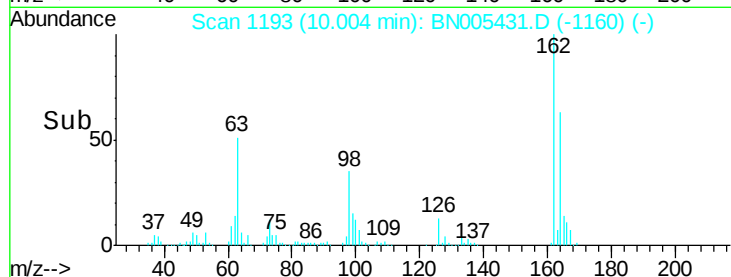
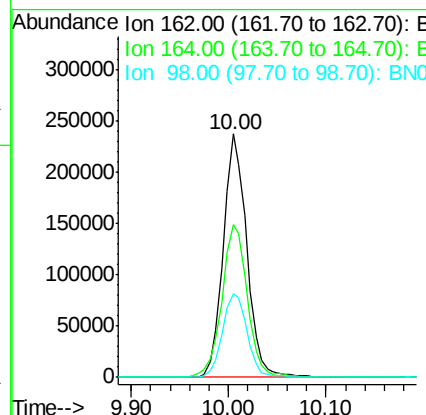


#27
 2,4-Dichlorophenol
 Concen: 21.835 ng/ul
 RT: 10.00 min Scan# 1193
 Delta R.T. -0.01 min
 Lab File: BN005431.D
 Acq: 03 May 2019 00:12

Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion:162 Resp: 397215
 Ion Ratio Lower Upper
 162 100
 164 62.9 52.6 79.0
 98 34.6 30.8 46.2

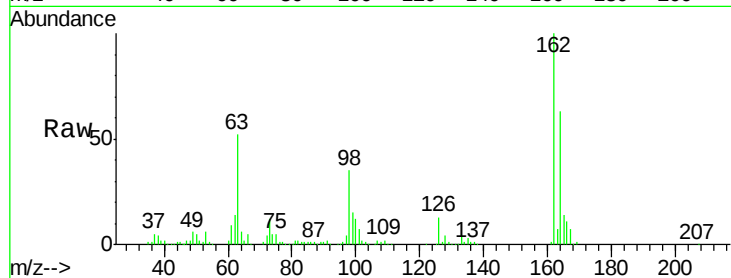

#28
 Naphthalene
 Concen: 20.099 ng/ul
 RT: 10.40 min Scan# 1260
 Delta R.T. -0.00 min
 Lab File: BN005431.D
 Acq: 03 May 2019 00:12

Tgt Ion:128 Resp: 1204175
 Ion Ratio Lower Upper
 128 100
 129 11.0 9.2 13.8
 127 12.9 10.7 16.1

