

#30

4-Chloroaniline

Concen: 22.748 ng/ul

RT: 10.52 min Scan# 1280

Delta R.T. -0.00 min

Lab File: BN005431.D

Acq: 03 May 2019 00:12

Instrument :

BNA_N


ClientSampled :

Tgt Ion:127 Resp: 440469

Ion Ratio Lower Upper




127 100

129 31.5 25.8 38.6

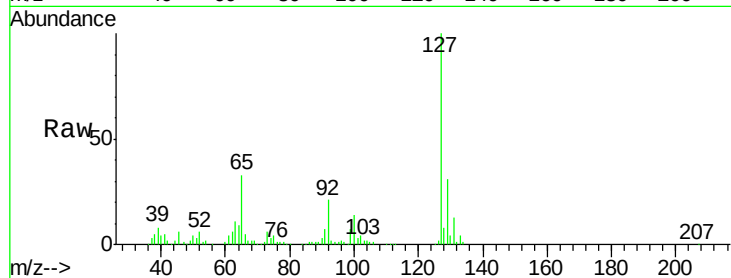

Abundance Ion 127.00 (126.70 to 127.70): E

Ion 129.00 (128.70 to 129.70): E

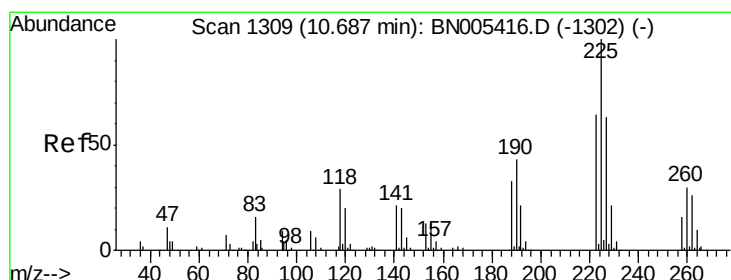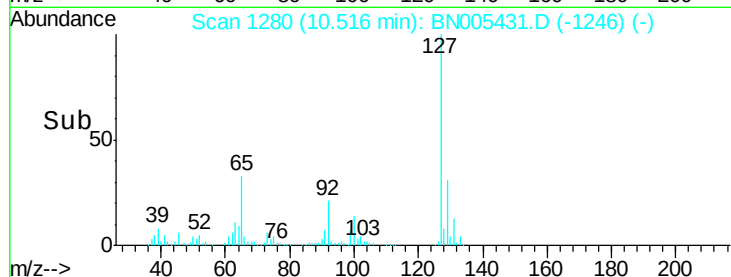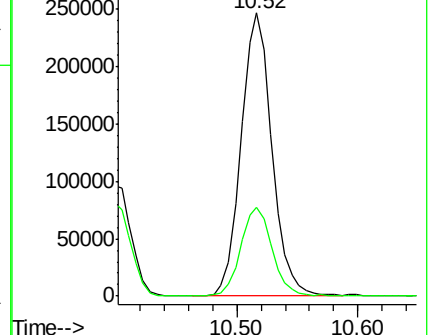

#31

Hexachlorobutadiene

Concen: 21.141 ng/ul

RT: 10.69 min Scan# 1309

Delta R.T. -0.00 min

Lab File: BN005431.D

Acq: 03 May 2019 00:12


Tgt Ion:225 Resp: 271593

Ion Ratio Lower Upper

225 100

223 62.1 48.5 72.7

227 64.1 51.0 76.6

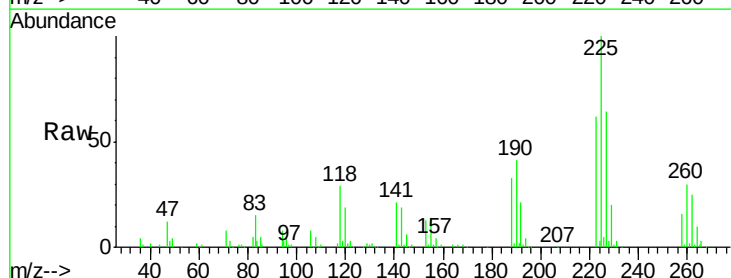

Abundance Ion 225.00 (224.70 to 225.70): E

Ion 223.00 (222.70 to 223.70): E

Ion 227.00 (226.70 to 227.70): E

