

#37

Hexachlorocyclopentadiene

Concen: 19.674 ng/ul

RT: 12.37 min Scan# 1596

Delta R.T. -0.00 min

Lab File: BN005431.D

Acq: 03 May 2019 00:12

Instrument :

BNA_N

ClientSampleId :


Tgt Ion: 237 Resp: 355421

Ion Ratio Lower Upper

237 100

235 63.7 51.1 76.7




272 13.7 9.5 14.3

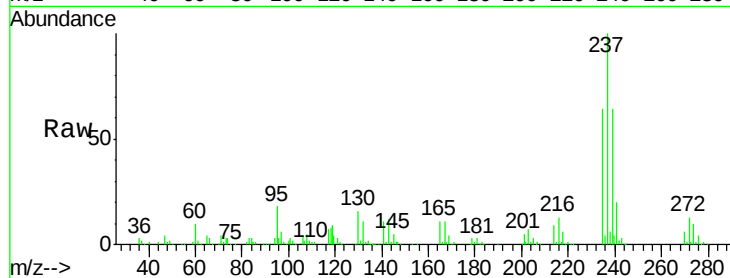

Abundance Ion 237.00 (236.70 to 237.70): E

Ion 235.00 (234.70 to 235.70): E

Ion 272.00 (271.70 to 272.70): E

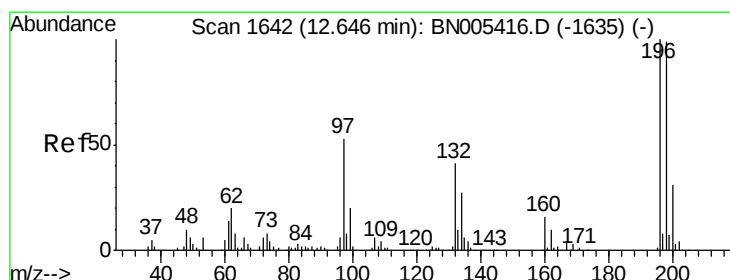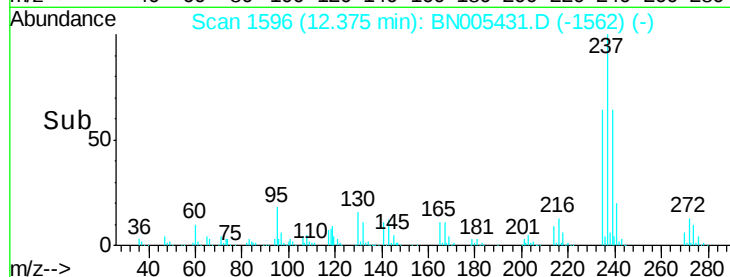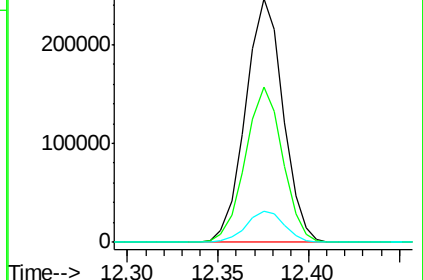

#38

2,4,6-Trichlorophenol

Concen: 21.735 ng/ul

RT: 12.65 min Scan# 1642

Delta R.T. -0.00 min

Lab File: BN005431.D

Acq: 03 May 2019 00:12


Tgt Ion: 196 Resp: 347279

Ion Ratio Lower Upper

196 100

198 94.6 74.8 112.2

200 32.3 23.5 35.3

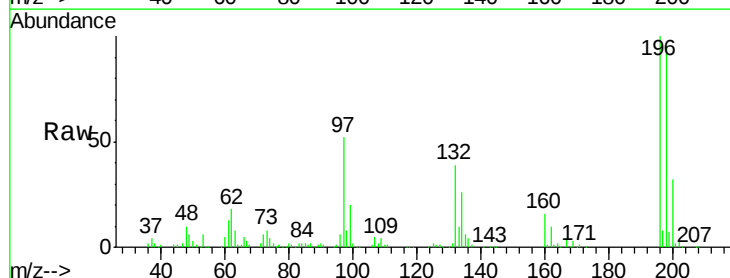

Abundance Ion 196.00 (195.70 to 196.70): E

Ion 198.00 (197.70 to 198.70): E

Ion 200.00 (199.70 to 200.70): E

