





#39
 2,4,5-Trichlorophenol
 Concen: 21.467 ng/ul
 RT: 12.72 min Scan# 1654
 Delta R.T. -0.00 min
 Lab File: BN005431.D
 Acq: 03 May 2019 00:12

Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion:196 Resp: 368567
 Ion Ratio Lower Upper
 196 100
 198 95.9 75.0 112.4
 200 31.2 24.2 36.4

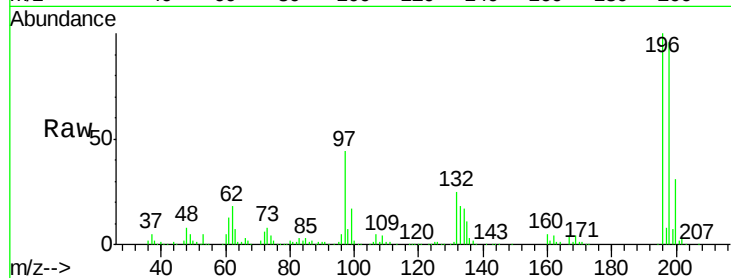


Abundance Ion 196.00 (195.70 to 196.70): E
 Ion 198.00 (197.70 to 198.70): E
 Ion 200.00 (199.70 to 200.70): E

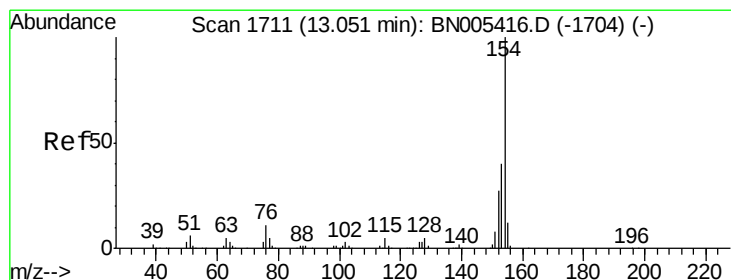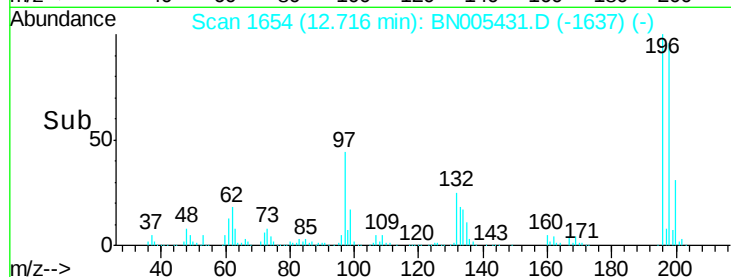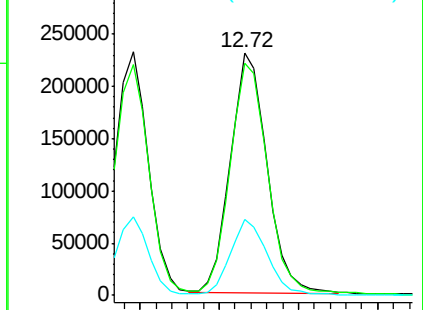

#40
 1,1'-Biphenyl
 Concen: 19.513 ng/ul
 RT: 13.05 min Scan# 1711
 Delta R.T. -0.00 min
 Lab File: BN005431.D
 Acq: 03 May 2019 00:12

Tgt Ion:154 Resp: 1244837
 Ion Ratio Lower Upper
 154 100
 153 40.1 32.6 49.0
 76 11.0 10.4 15.6

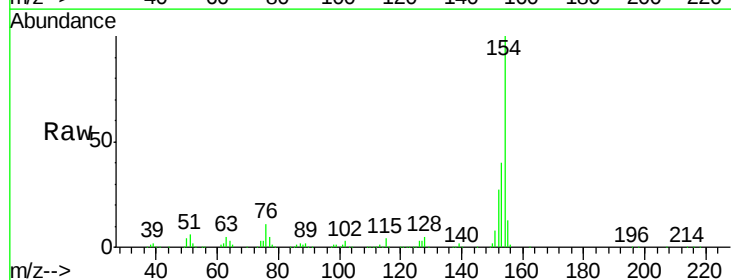

Abundance Ion 154.00 (153.70 to 154.70): E
 Ion 153.00 (152.70 to 153.70): E
 Ion 76.00 (75.70 to 76.70): BNC

