

#47

Acenaphthylene

Concen: 20.243 ng/ul

RT: 13.95 min Scan# 1863

Delta R.T. -0.00 min

Lab File: BN005431.D

Acq: 03 May 2019 00:12

Instrument :

BNA_N

ClientSampleId :


Tgt Ion:152 Resp: 1518611

Ion Ratio Lower Upper

152 100

151 19.9 15.8 23.8




153 12.8 9.8 14.8

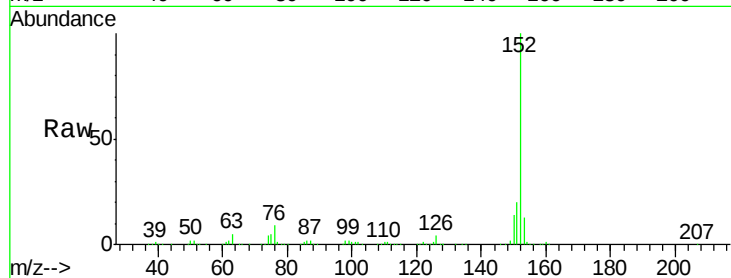

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

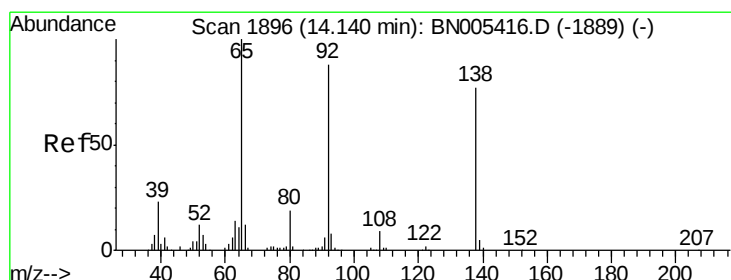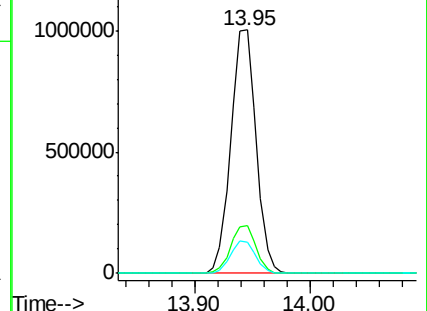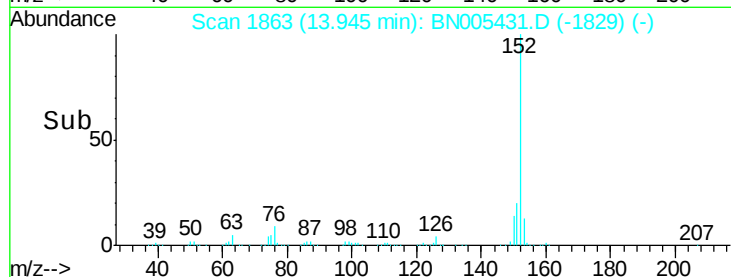

#48

3-Nitroaniline

Concen: 24.288 ng/ul

RT: 14.14 min Scan# 1896

Delta R.T. -0.00 min

Lab File: BN005431.D

Acq: 03 May 2019 00:12


Tgt Ion:138 Resp: 241451

Ion Ratio Lower Upper

138 100

108 11.8 12.1 18.1#

92 118.6 102.9 154.3

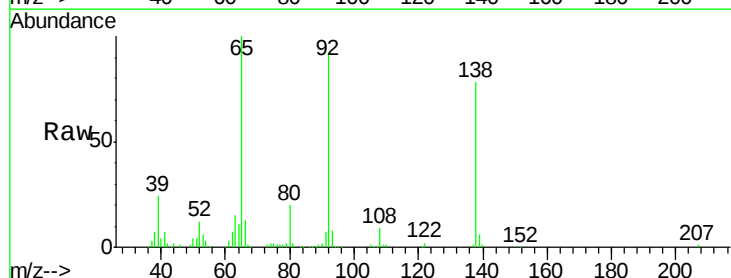

Abundance Ion 138.00 (137.70 to 138.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 92.00 (91.70 to 92.70): BNC

