





#65
 4-Bromophenyl-phenylether
 Concen: 20.982 ng/ul
 RT: 16.17 min Scan# 2242
 Delta R.T. -0.01 min
 Lab File: BN005431.D
 Acq: 03 May 2019 00:12

Instrument :
 BNA_N
 ClientSampled :

Tgt Ion:248 Resp: 428111
 Ion Ratio Lower Upper
 248 100
 250 101.3 78.4 117.6
 141 70.8 61.8 92.6

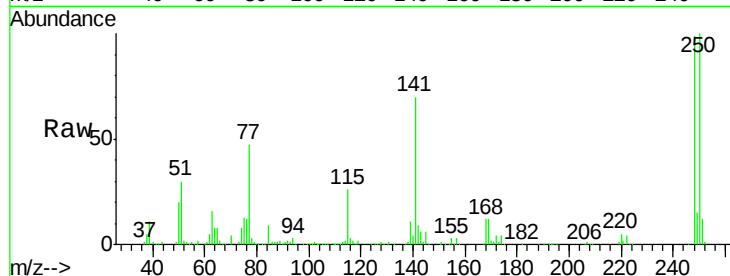


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

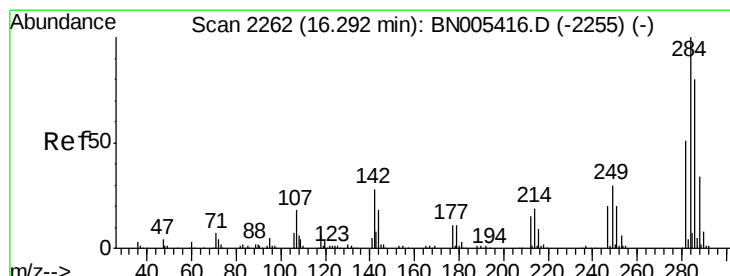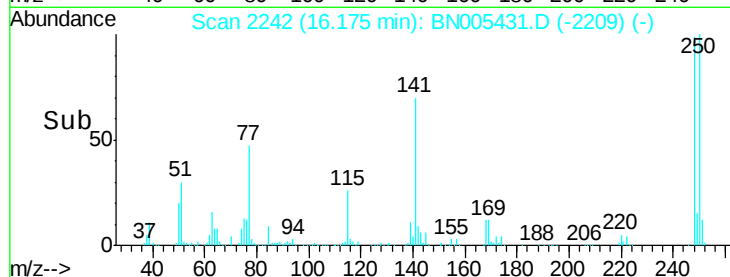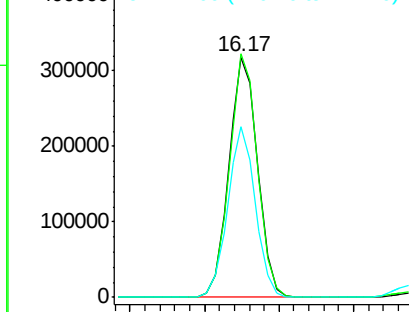

#66
 Hexachlorobenzene
 Concen: 21.507 ng/ul
 RT: 16.29 min Scan# 2261
 Delta R.T. -0.01 min
 Lab File: BN005431.D
 Acq: 03 May 2019 00:12

Tgt Ion:284 Resp: 467274
 Ion Ratio Lower Upper
 284 100
 142 30.3 29.4 44.2
 249 31.3 26.1 39.1

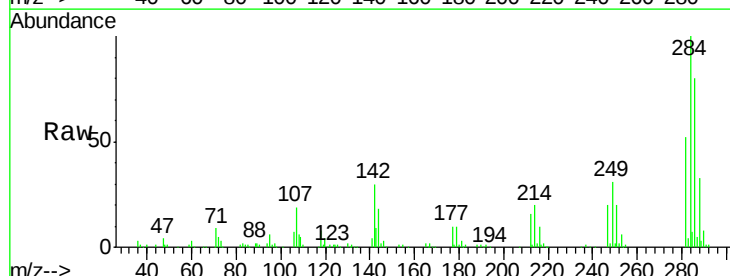

Abundance Ion 284.00 (283.70 to 284.70): E
 Ion 142.00 (141.70 to 142.70): E
 Ion 249.00 (248.70 to 249.70): E

