

#67

Atrazine

Concen: 20.897 ng/ul

RT: 16.46 min Scan# 2290

Delta R.T. -0.00 min

Lab File: BN005431.D

Acq: 03 May 2019 00:12

Instrument :

BNA_N

ClientSampleId :


Tgt Ion:200 Resp: 431223

Ion Ratio Lower Upper

200 100

173 26.3 21.4 32.0


215 50.2 39.1 58.7

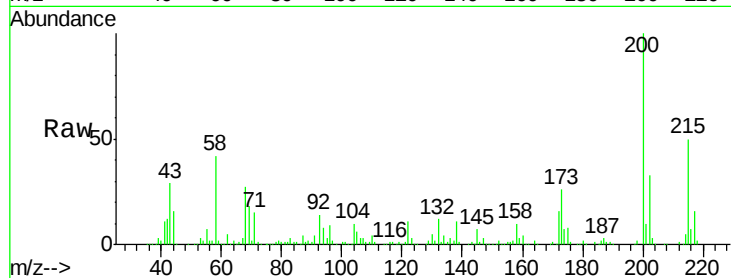



Abundance Ion 200.00 (199.70 to 200.70): E

Ion 173.00 (172.70 to 173.70): E

Ion 215.00 (214.70 to 215.70): E

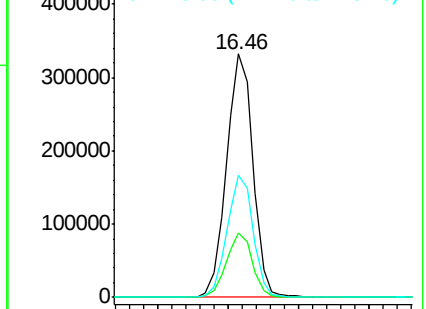

Time-->

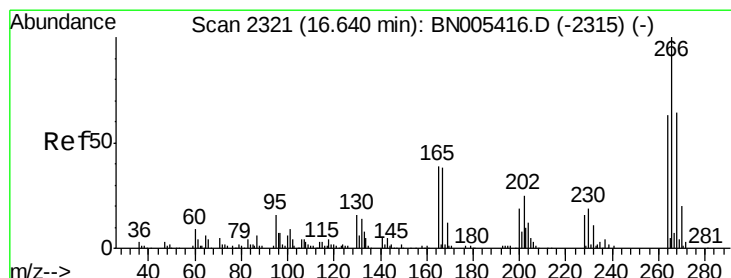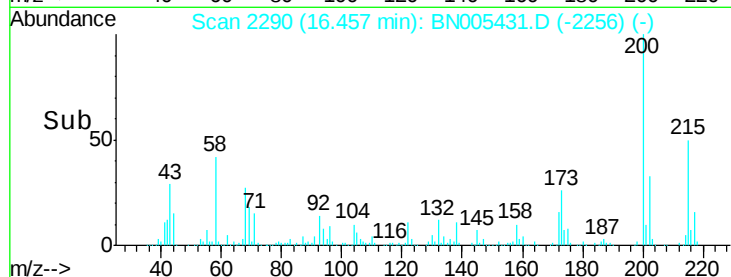

#68

Pentachlorophenol

Concen: 20.567 ng/ul

RT: 16.63 min Scan# 2320

Delta R.T. -0.01 min

Lab File: BN005431.D

Acq: 03 May 2019 00:12


Tgt Ion:266 Resp: 261638

Ion Ratio Lower Upper

266 100

264 61.5 49.7 74.5


268 62.8 52.4 78.6

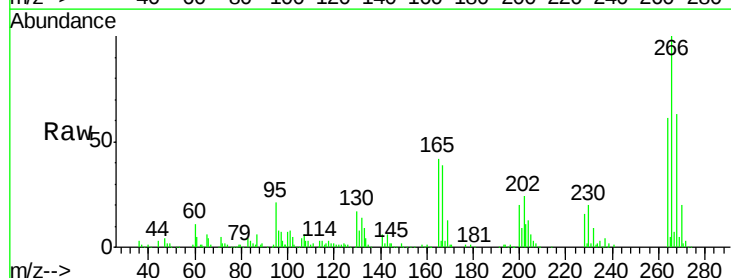

Abundance Ion 265.70 (265.40 to 266.40): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

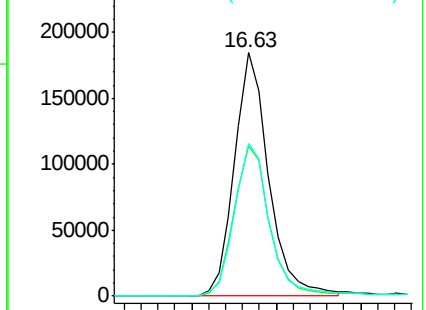

Time-->

