





#80
Butylbenzylphthalate
Concen: 20.828 ng/ul
RT: 20.35 min Scan# 2952
Delta R.T. -0.00 min
Lab File: BN005431.D
Acq: 03 May 2019 00:12

Instrument :
BNA_N
ClientSampleId :

Tgt Ion	Ratio	Lower	Upper
149	100		
91	65.8	59.6	89.4
206	24.4	17.8	26.8

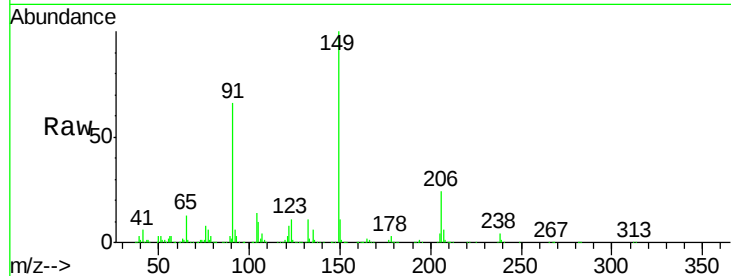


Abundance Ion 149.00 (148.70 to 149.70): E
Ion 91.00 (90.70 to 91.70): BNO
Ion 206.00 (205.70 to 206.70): E

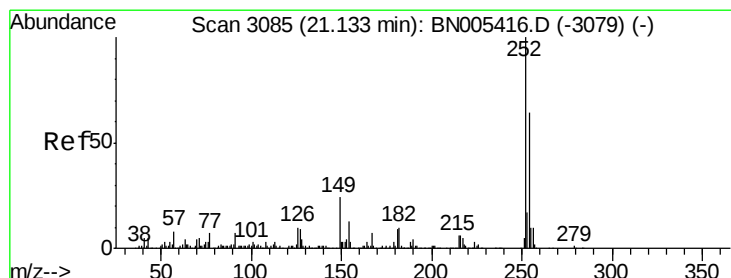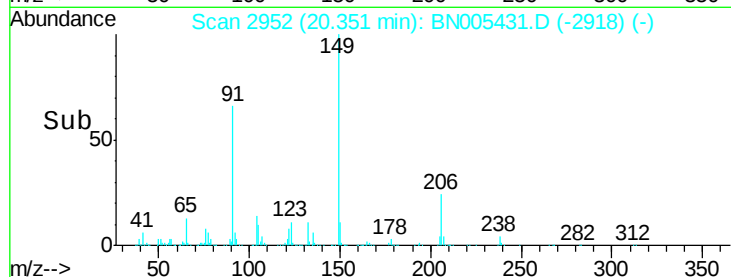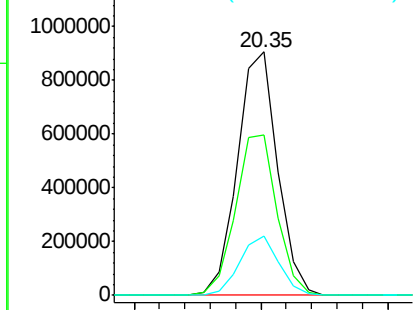

#81
3,3'-Dichlorobenzidine
Concen: 19.923 ng/ul
RT: 21.13 min Scan# 3085
Delta R.T. -0.00 min
Lab File: BN005431.D
Acq: 03 May 2019 00:12

Tgt Ion	Ratio	Lower	Upper
252	100		
254	63.9	51.1	76.7
126	8.8	9.4	14.0

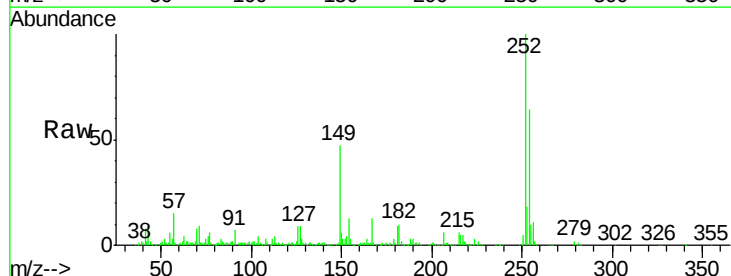

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 254.00 (253.70 to 254.70): E
Ion 126.00 (125.70 to 126.70): E

