

#82

Benzo(a)anthracene

Concen: 20.136 ng/ul

RT: 21.19 min Scan# 3095

Delta R.T. -0.01 min

Lab File: BN005431.D

Acq: 03 May 2019 00:12

Instrument :

BNA_N

ClientSampleId :


Tgt Ion:228 Resp: 2345819

Ion Ratio Lower Upper

228 100

229 19.9 15.8 23.6




226 26.6 21.4 32.2

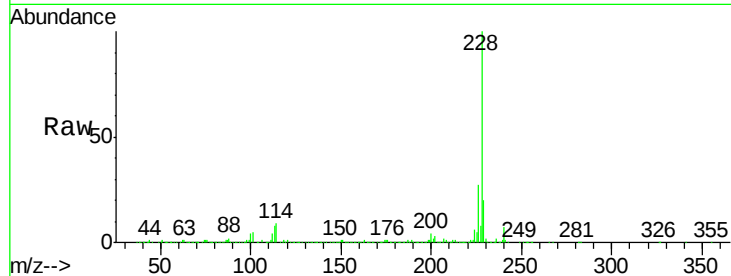

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

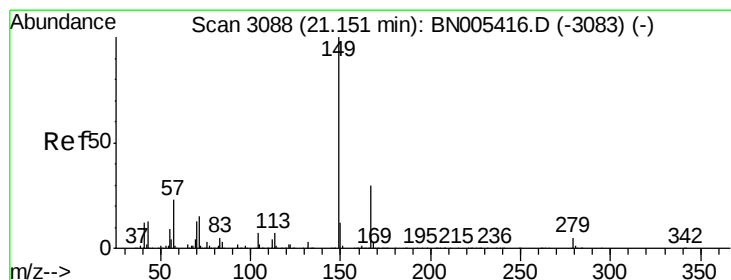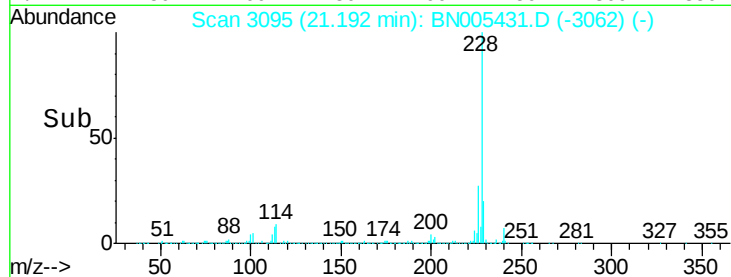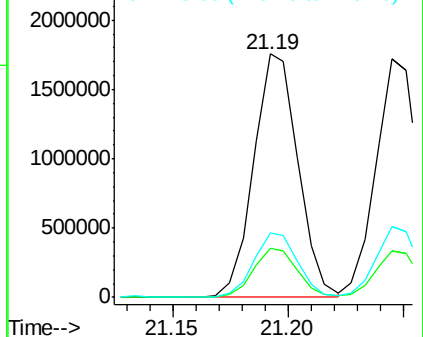

#83

Bis(2-ethylhexyl)phthalate

Concen: 19.524 ng/ul

RT: 21.15 min Scan# 3087

Delta R.T. -0.01 min

Lab File: BN005431.D

Acq: 03 May 2019 00:12


Tgt Ion:149 Resp: 1435161

Ion Ratio Lower Upper

149 100

167 29.3 22.3 33.5

279 4.8 3.3 4.9

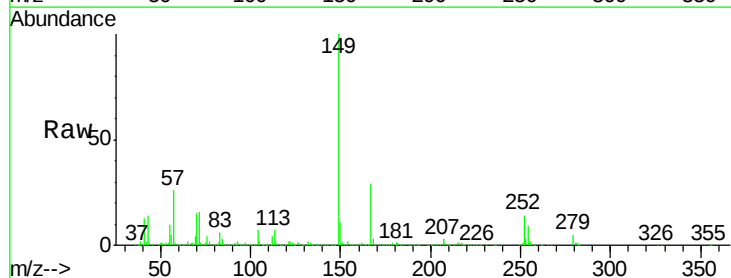

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

