


#92




Dibenzo(a,h)anthracene
 Concen: 18.324 ng/ul
 RT: 25.62 min Scan# 3847
 Delta R.T. -0.01 min
 Lab File: BN005431.D
 Acq: 03 May 2019 00:12

Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion: 278 Resp: 1615890
 Ion Ratio Lower Upper
 278 100
 139 13.3 13.1 19.7
 279 23.3 19.4 29.0

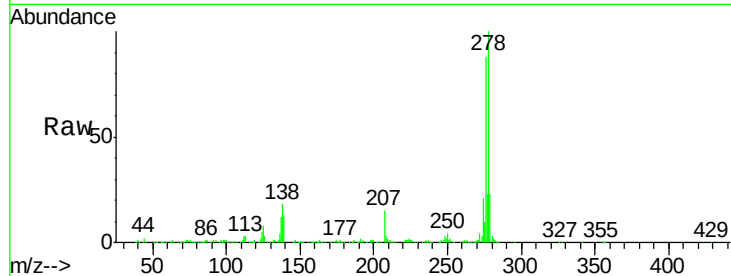


Abundance Ion 278.00 (277.70 to 278.70): E
 Ion 139.00 (138.70 to 139.70): E
 Ion 279.00 (278.70 to 279.70): E

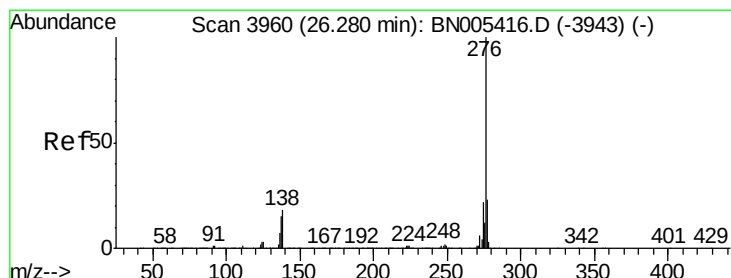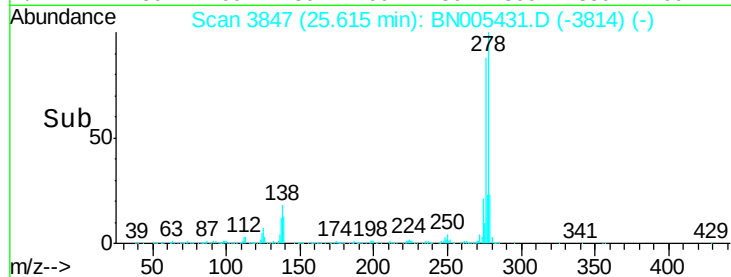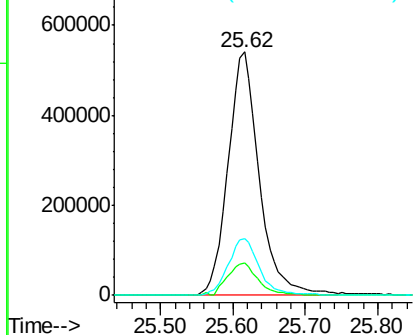

#93

Benzo(g,h,i)perylene
 Concen: 17.990 ng/ul
 RT: 26.27 min Scan# 3958
 Delta R.T. -0.01 min
 Lab File: BN005431.D
 Acq: 03 May 2019 00:12

Tgt Ion: 276 Resp: 1545673
 Ion Ratio Lower Upper
 276 100
 138 17.0 16.7 25.1
 277 23.4 18.2 27.2

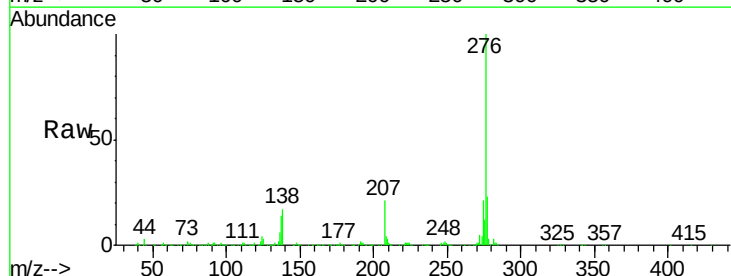

Abundance Ion 276.00 (275.70 to 276.70): E
 Ion 138.00 (137.70 to 138.70): E
 Ion 277.00 (276.70 to 277.70): E

