

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050225\
 Data File : BN036957.D
 Acq On : 02 May 2025 13:55
 Operator : RC/JU
 Sample : PB166547BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK547

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041525.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN036957.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.111	34	38	46	rVB	27360	38838	1.94%	0.161%
2	3.517	103	107	130	rBV	404212	661122	32.94%	2.744%
3	3.834	157	161	167	rBV2	7061	11758	0.59%	0.049%
4	6.799	658	665	678	rBV	556654	825776	41.15%	3.427%
5	6.963	687	693	703	rVB	354078	537897	26.80%	2.233%
6	7.158	720	726	738	rVB	510938	758521	37.80%	3.148%
7	7.622	798	805	816	rVB	363033	556926	27.75%	2.312%
8	8.334	919	926	935	rBV	607472	918315	45.76%	3.812%
9	8.775	994	1001	1013	rBV	476028	748245	37.29%	3.106%
10	8.905	1018	1023	1028	rVB4	5441	8483	0.42%	0.035%
11	9.210	1070	1075	1080	rVB4	1521	2063	0.10%	0.009%
12	9.493	1117	1123	1135	rVB	407390	634944	31.64%	2.635%
13	10.028	1208	1214	1222	rBV	568416	907177	45.21%	3.765%
14	10.404	1271	1278	1285	rBV	460720	746190	37.18%	3.097%
15	10.546	1295	1302	1316	rBV	568590	902381	44.97%	3.745%
16	12.010	1546	1551	1557	rBV3	5312	9121	0.45%	0.038%
17	13.693	1831	1837	1845	rBV	965930	1292871	64.43%	5.366%
18	13.963	1877	1883	1894	rBV	948002	1380334	68.78%	5.729%
19	14.275	1930	1936	1943	rBV	690475	980101	48.84%	4.068%
20	14.481	1965	1971	1982	rBV	542529	774163	38.58%	3.213%
21	15.269	2099	2105	2115	rBV	1208862	1684816	83.96%	6.993%
22	15.392	2120	2126	2134	rBV	578169	725131	36.13%	3.010%
23	15.510	2143	2146	2150	rBV3	3982	5162	0.26%	0.021%
24	16.810	2362	2367	2371	rVB3	2595	3022	0.15%	0.013%
25	17.022	2397	2403	2411	rBV2	850867	1128985	56.26%	4.686%
26	17.122	2413	2420	2430	rBV	1385884	1839767	91.68%	7.636%
27	17.928	2553	2557	2560	rBV2	14716	17369	0.87%	0.072%
28	18.986	2733	2737	2741	rBV5	11644	16148	0.80%	0.067%
29	19.057	2745	2749	2753	rBV2	10535	14085	0.70%	0.058%
30	19.216	2773	2776	2779	rBV4	7430	7825	0.39%	0.032%
31	19.422	2805	2811	2819	rBV	1554795	2006761	100.00%	8.329%
32	21.251	3116	3122	3129	rBV	854500	1149299	57.27%	4.770%
33	23.945	3572	3580	3595	rVB	730677	1692478	84.34%	7.025%
34	24.139	3605	3613	3628	rVB2	448863	1106925	55.16%	4.594%

Sum of corrected areas: 24092999

Instrument :

BNA_N

ClientSampleId :




SBLK547

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050225\
Data File : BN036957.D
Acq On : 02 May 2025 13:55
Operator : RC/JU
Sample : PB166547BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK547

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041525.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

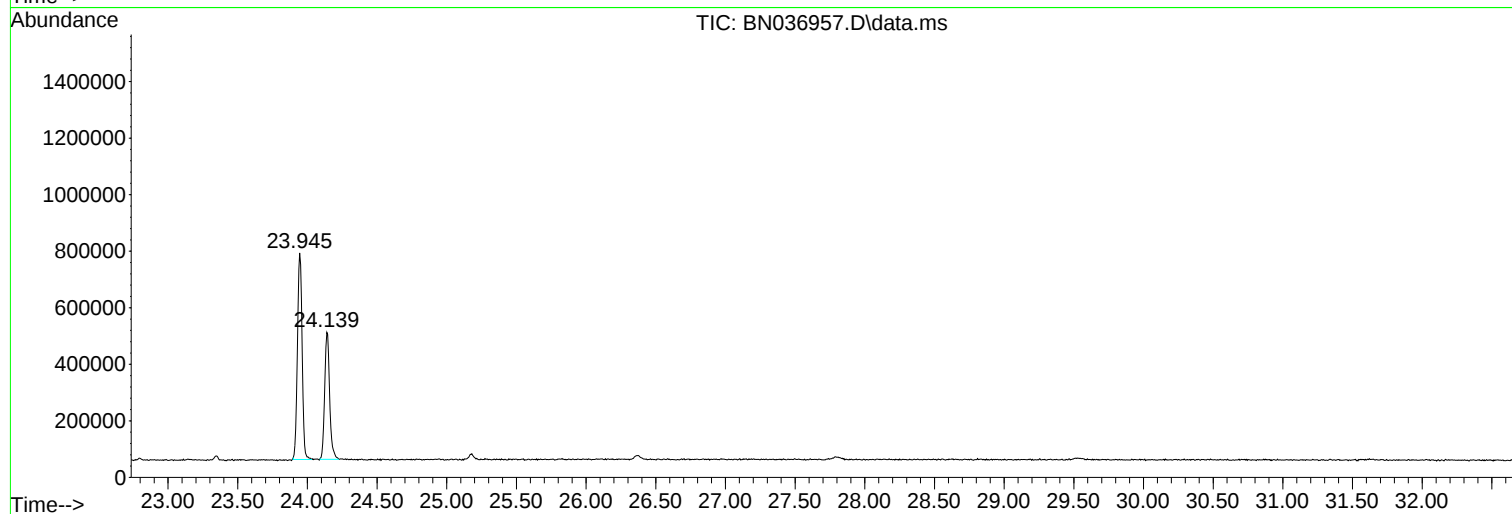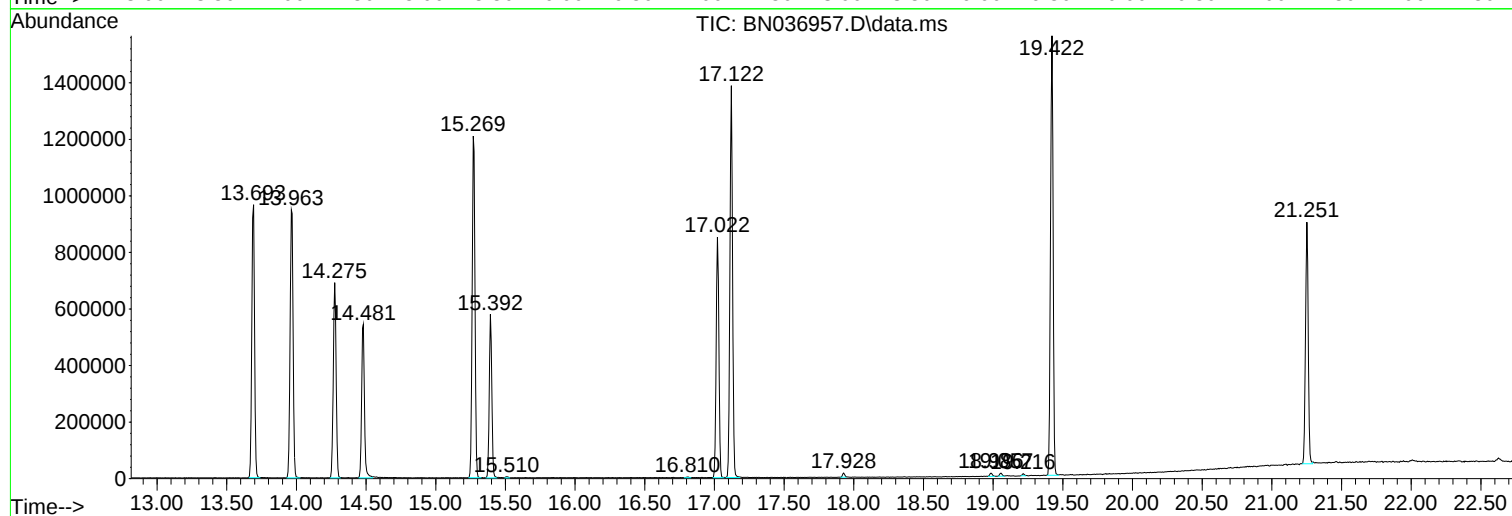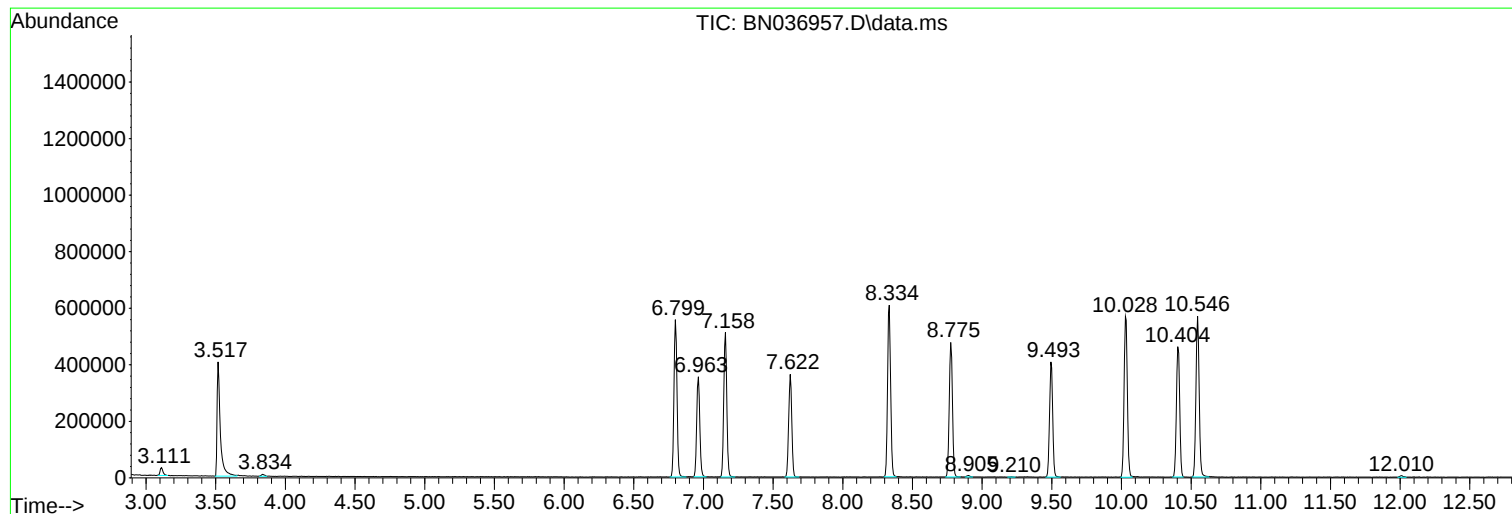

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050225\
Data File : BN036957.D
Acq On : 02 May 2025 13:55
Operator : RC/JU
Sample : PB166547BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK547

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041525.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050225\
Data File : BN036957.D
Acq On : 02 May 2025 13:55
Operator : RC/JU
Sample : PB166547BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK547

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041525.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc