

Data File : BN005500.D  
 Acq On : 06 May 2019 23:56  
 Operator : JU/SJ  
 Sample : K2470-04  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 A5135

Quant Time: May 07 07:09:10 2019  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN050719.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue May 07 07:04:57 2019  
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	1563	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.35	136	6397	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.23	164	4144	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.08	188	648880	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.23
20) Perylene-d12	23.28	264	785177	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.97	152	2926	0.29	ng/ul	-0.02
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
8) Acenaphthene	14.29	153	525	0.036	ng/ul	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN005500.D  
Acq On : 06 May 2019 23:56  
Operator : JU/SJ  
Sample : K2470-04  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
A5135

Quant Time: May 07 07:09:10 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN050719.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue May 07 07:04:57 2019  
Response via : Initial Calibration

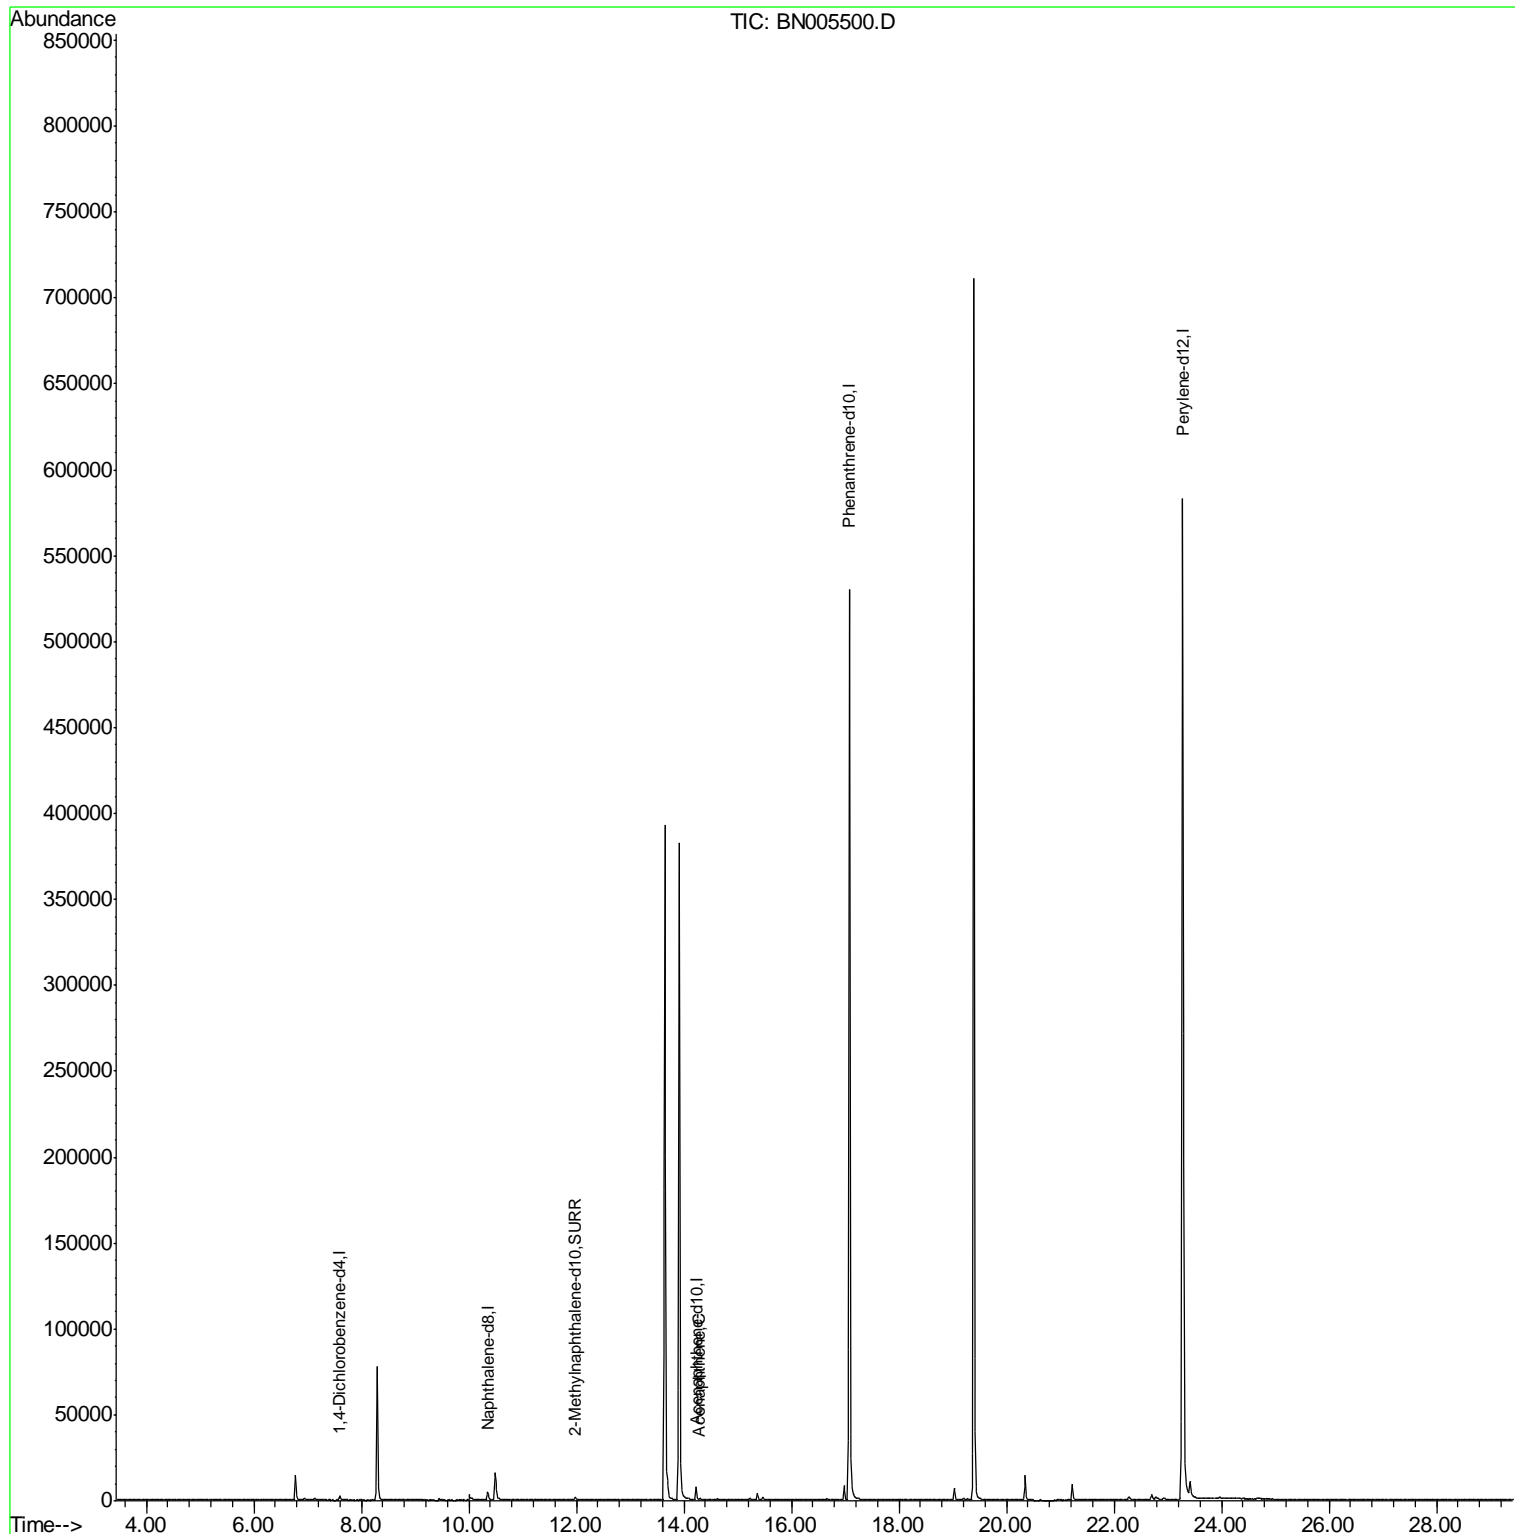

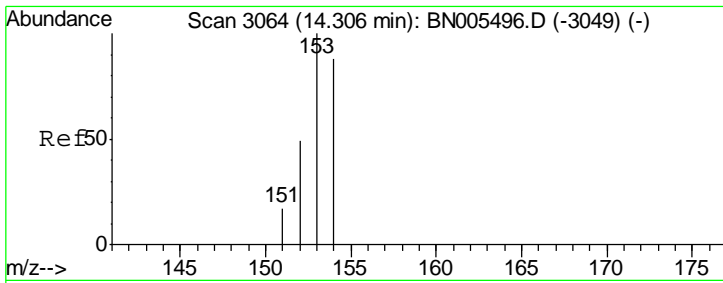

#8  
 Acenaphthene  
 Concen: 0.036 ng/ul  
 RT: 14.29 min Scan# 3060  
 Delta R.T. -0.02 min  
 Lab File: BN005500.D  
 Acq: 06 May 2019 23:56

Instrument :  
 BNA\_N  
 ClientSampled :  
 A5135

Tgt Ion	Resp	Lower	Upper
153	525		
152	54.6	40.8	61.2
154	90.5	73.2	109.8

