

Data File : BN005501.D
Acq On : 07 May 2019 00:30
Operator : JU/SJ
Sample : K2470-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5135

Quant Time: May 07 07:09:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 07 07:04:57 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	1764	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.35	136	7033	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.22	164	4583	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.08	188	789068	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.23
20) Perylene-d12	23.28	264	922346	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.96	152	3576	0.32	ng/ul	-0.03
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
8) Acenaphthene	14.29	153	458496	28.083	ng/ul	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN005501.D
Acq On : 07 May 2019 00:30
Operator : JU/SJ
Sample : K2470-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5135

Quant Time: May 07 07:09:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 07 07:04:57 2019
Response via : Initial Calibration

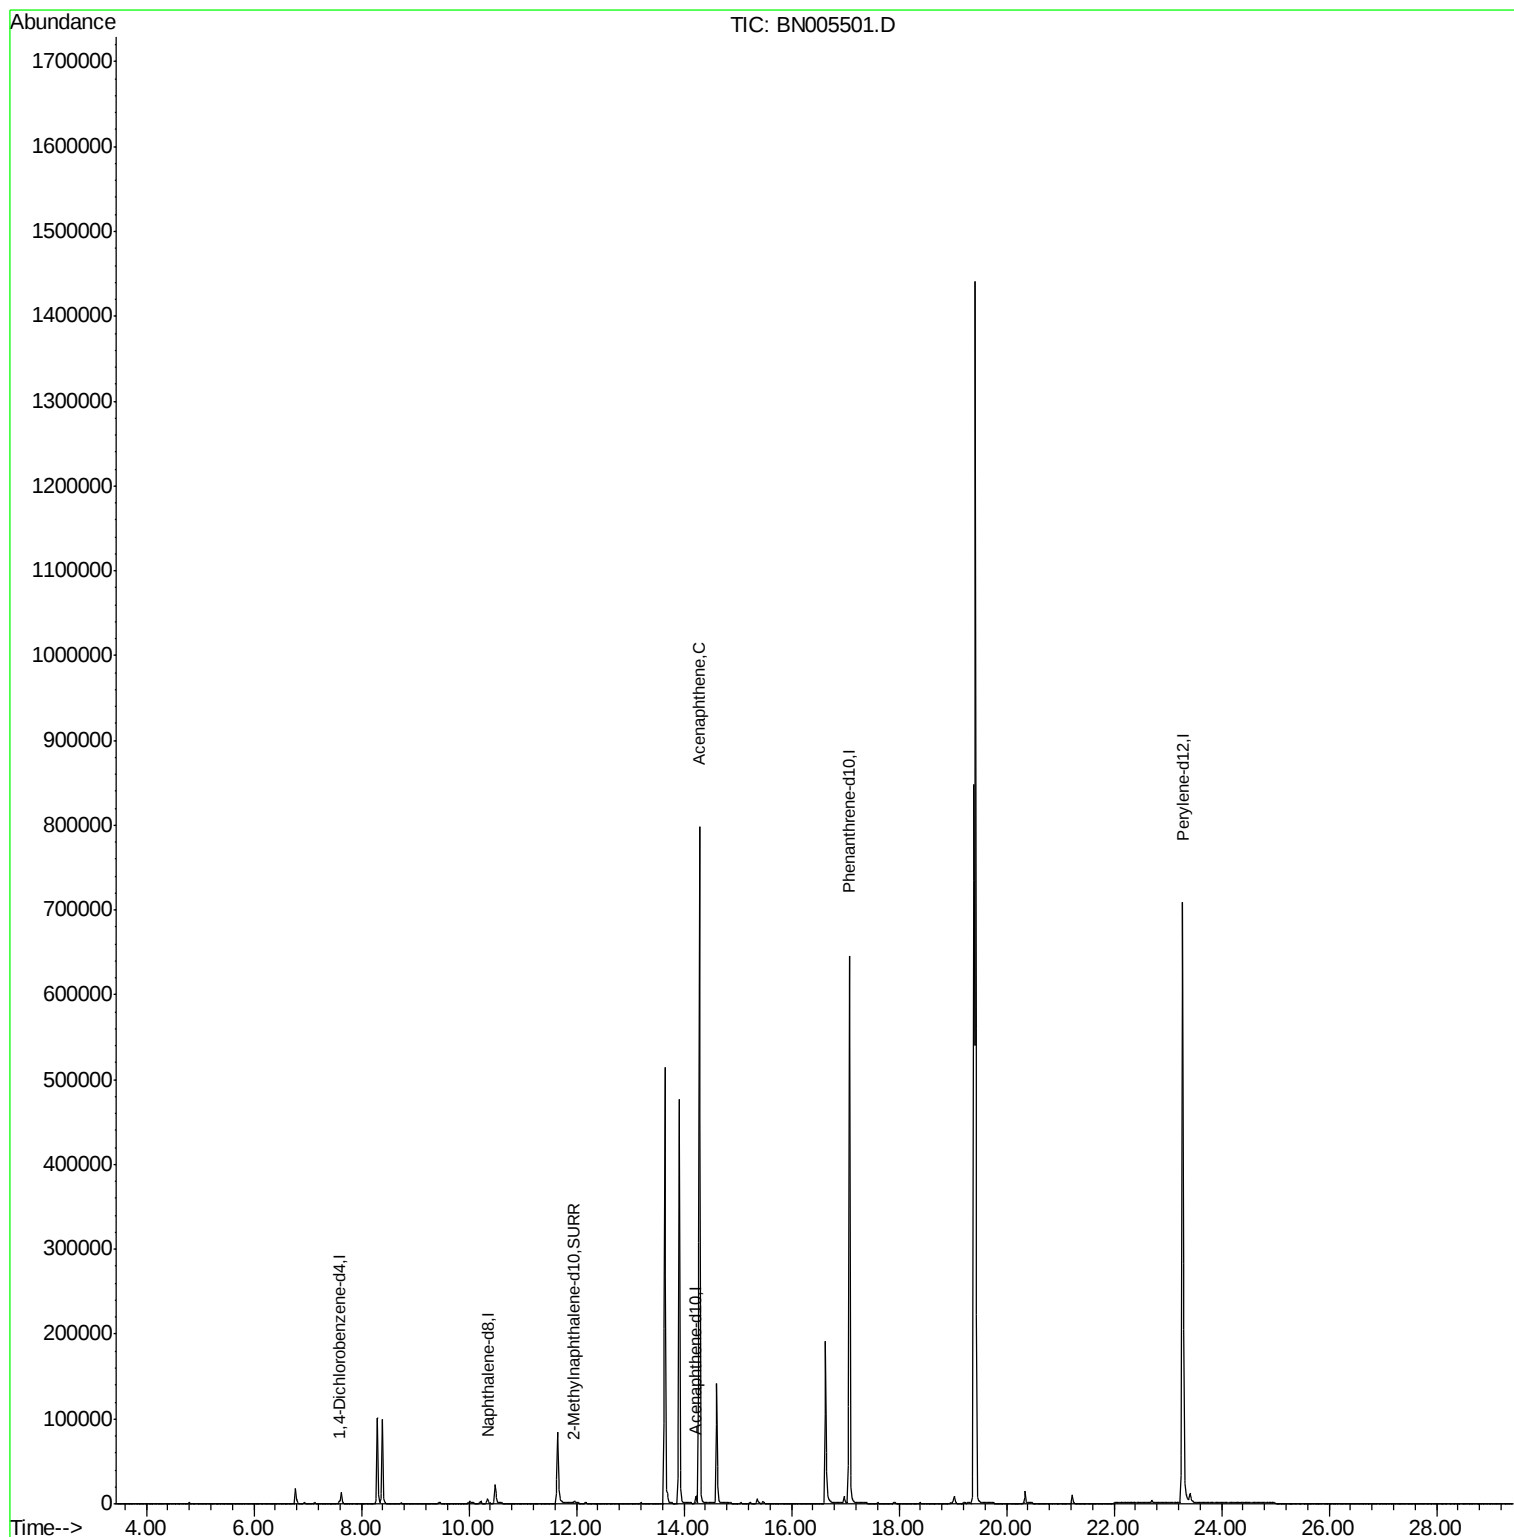

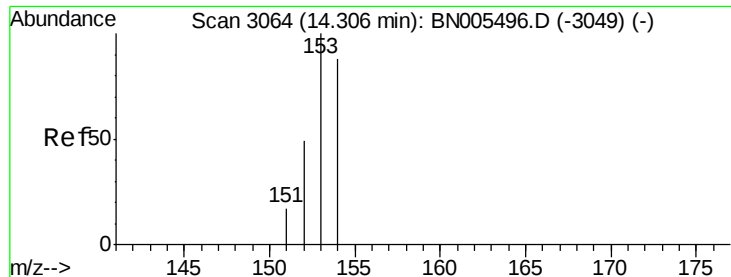

#8

Acenaphthene

Concen: 28.083 ng/ul

RT: 14.29 min Scan# 3060

Delta R.T. -0.02 min

Lab File: BN005501.D

Acq: 07 May 2019 00:30

Instrument :

BNA_N

ClientSampleId :

A5135

Tgt Ion:153 Resp: 458496

Ion Ratio Lower Upper

153 100

152 47.3 40.8 61.2

154 89.8 73.2 109.8

