

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN050719\
Quantitation Report (Not Reviewed)

Data File : BN005505.D
Acq On : 07 May 2019 02:48
Operator : JU/SJ
Sample : K2403-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5103

Quant Time: May 07 07:09:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 07 07:04:57 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	2306	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.35	136	9192	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.22	164	6041	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.08	188	1148688	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.23
20) Perylene-d12	23.28	264	1235383	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.97	152	5224	0.36	ng/ul	-0.02
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.23	166	1765	0.070	ng/ul#	Qvalue 16




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN005505.D
Acq On : 07 May 2019 02:48
Operator : JU/SJ
Sample : K2403-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5103

Quant Time: May 07 07:09:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 07 07:04:57 2019
Response via : Initial Calibration

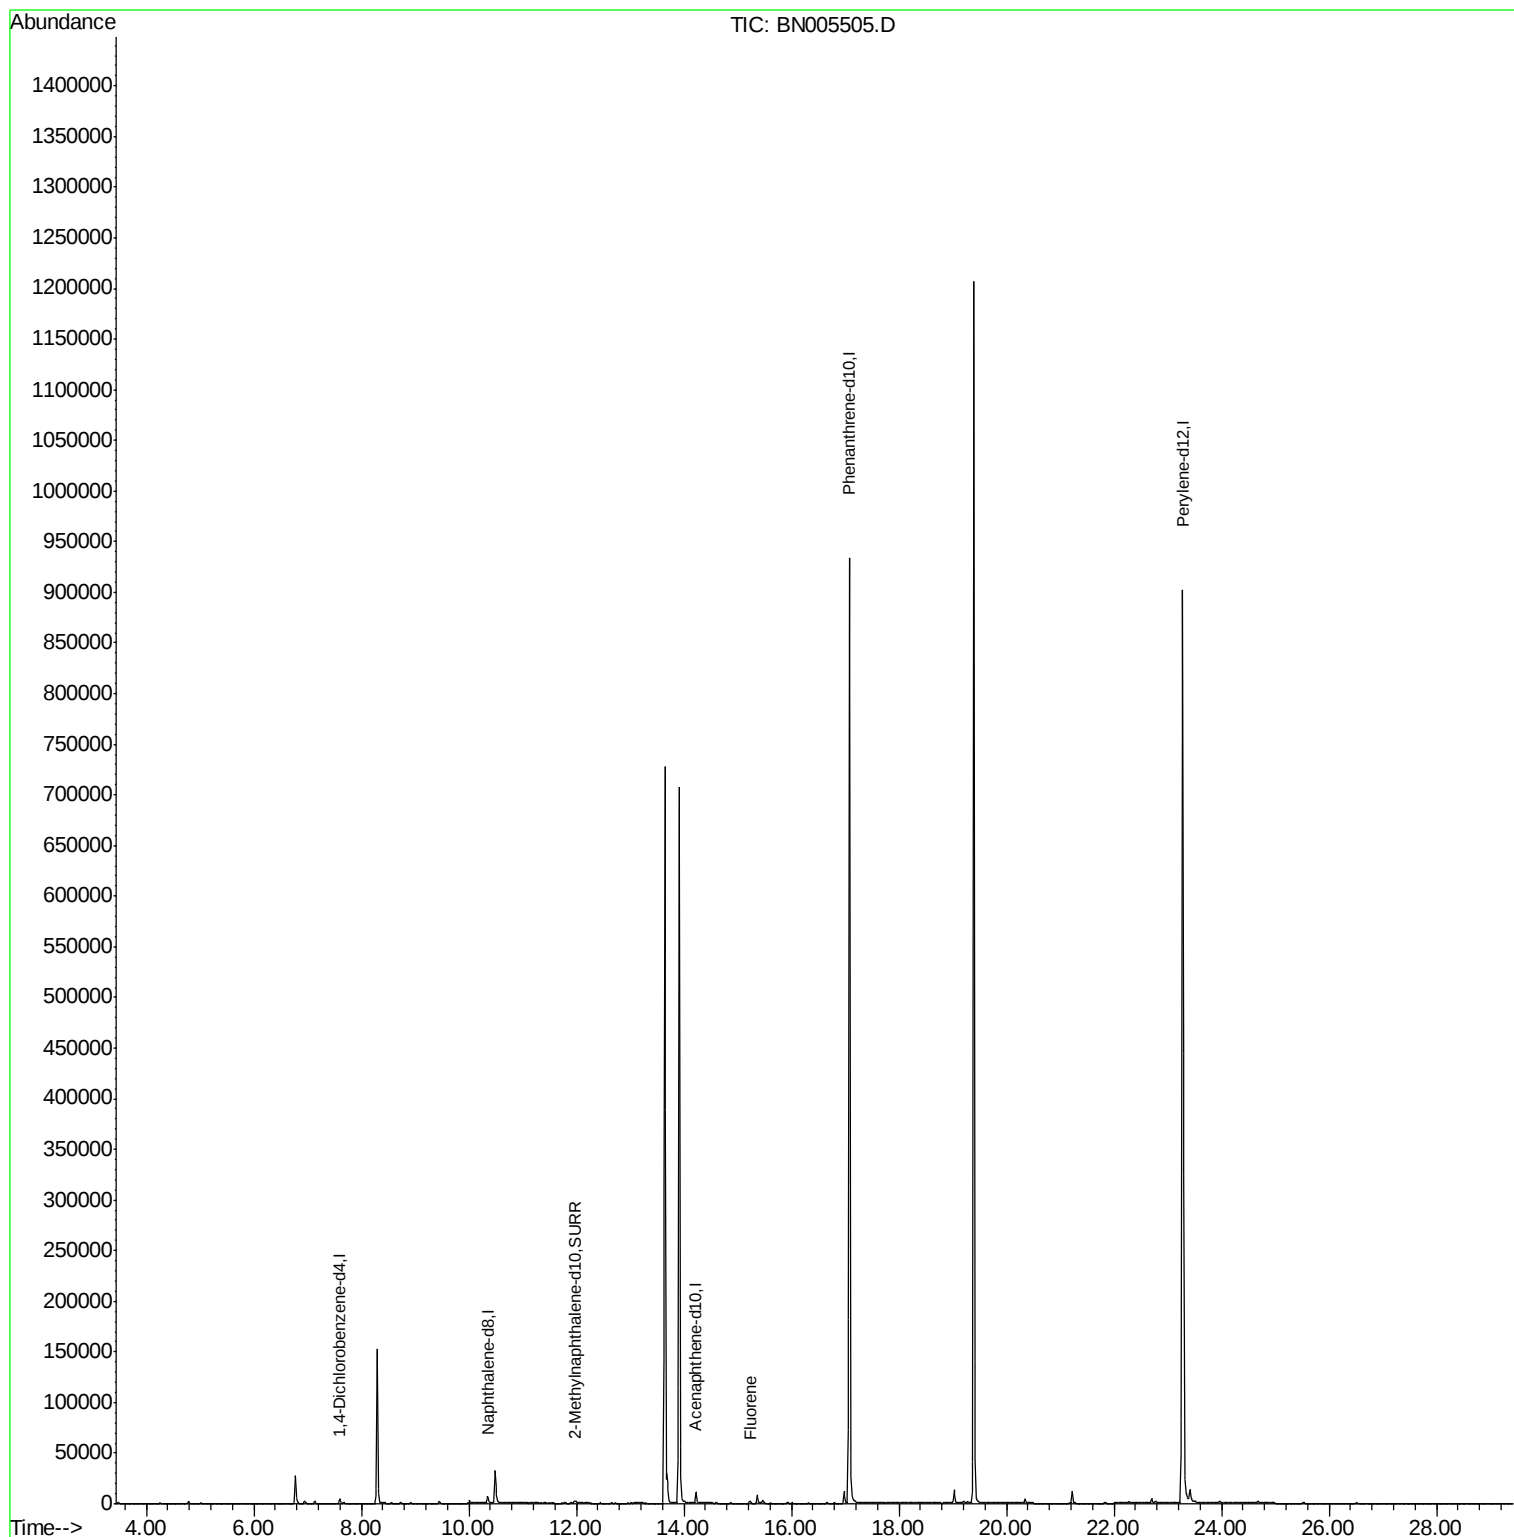

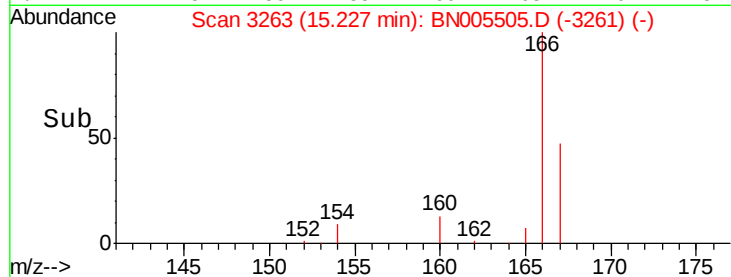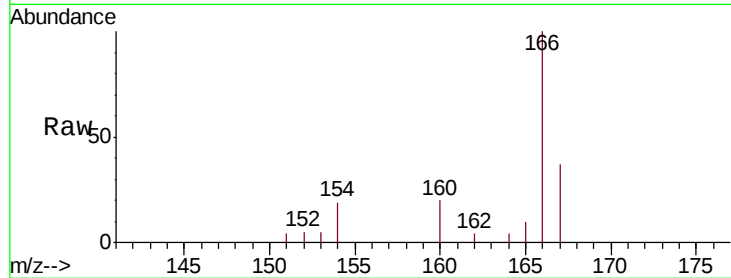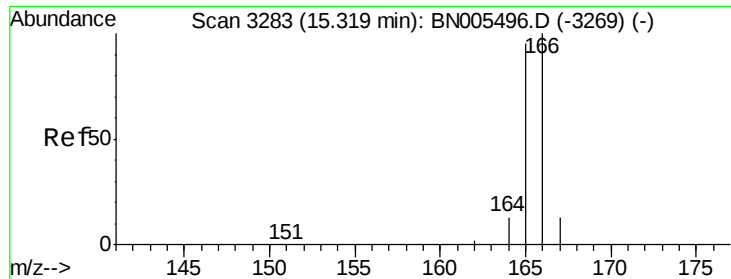

#9

Fluorene

Concen: 0.070 ng/ul

RT: 15.23 min Scan# 3263

Delta R.T. -0.09 min

Lab File: BN005505.D

Acq: 07 May 2019 02:48

Instrument :

BNA_N

ClientSampleId :

A5103

Tgt Ion:166 Resp: 1765

Ion Ratio Lower Upper

166 100

165 9.5 78.0 117.0#

167 36.7 12.2 18.4#

