

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN050719\
Quantitation Report (Not Reviewed)

Data File : BN005509.D
Acq On : 07 May 2019 05:05
Operator : JU/SJ
Sample : K2403-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5127

Quant Time: May 07 07:09:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 07 07:04:57 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	2265	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.35	136	9107	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.22	164	6029	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.08	188	1244387	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.23
20) Perylene-d12	23.28	264	1271198	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.96	152	5895	0.41	ng/ul	-0.03
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.23	166	1937	0.077	ng/ul#	16


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN005509.D
Acq On : 07 May 2019 05:05
Operator : JU/SJ
Sample : K2403-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5127

Quant Time: May 07 07:09:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN050719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 07 07:04:57 2019
Response via : Initial Calibration

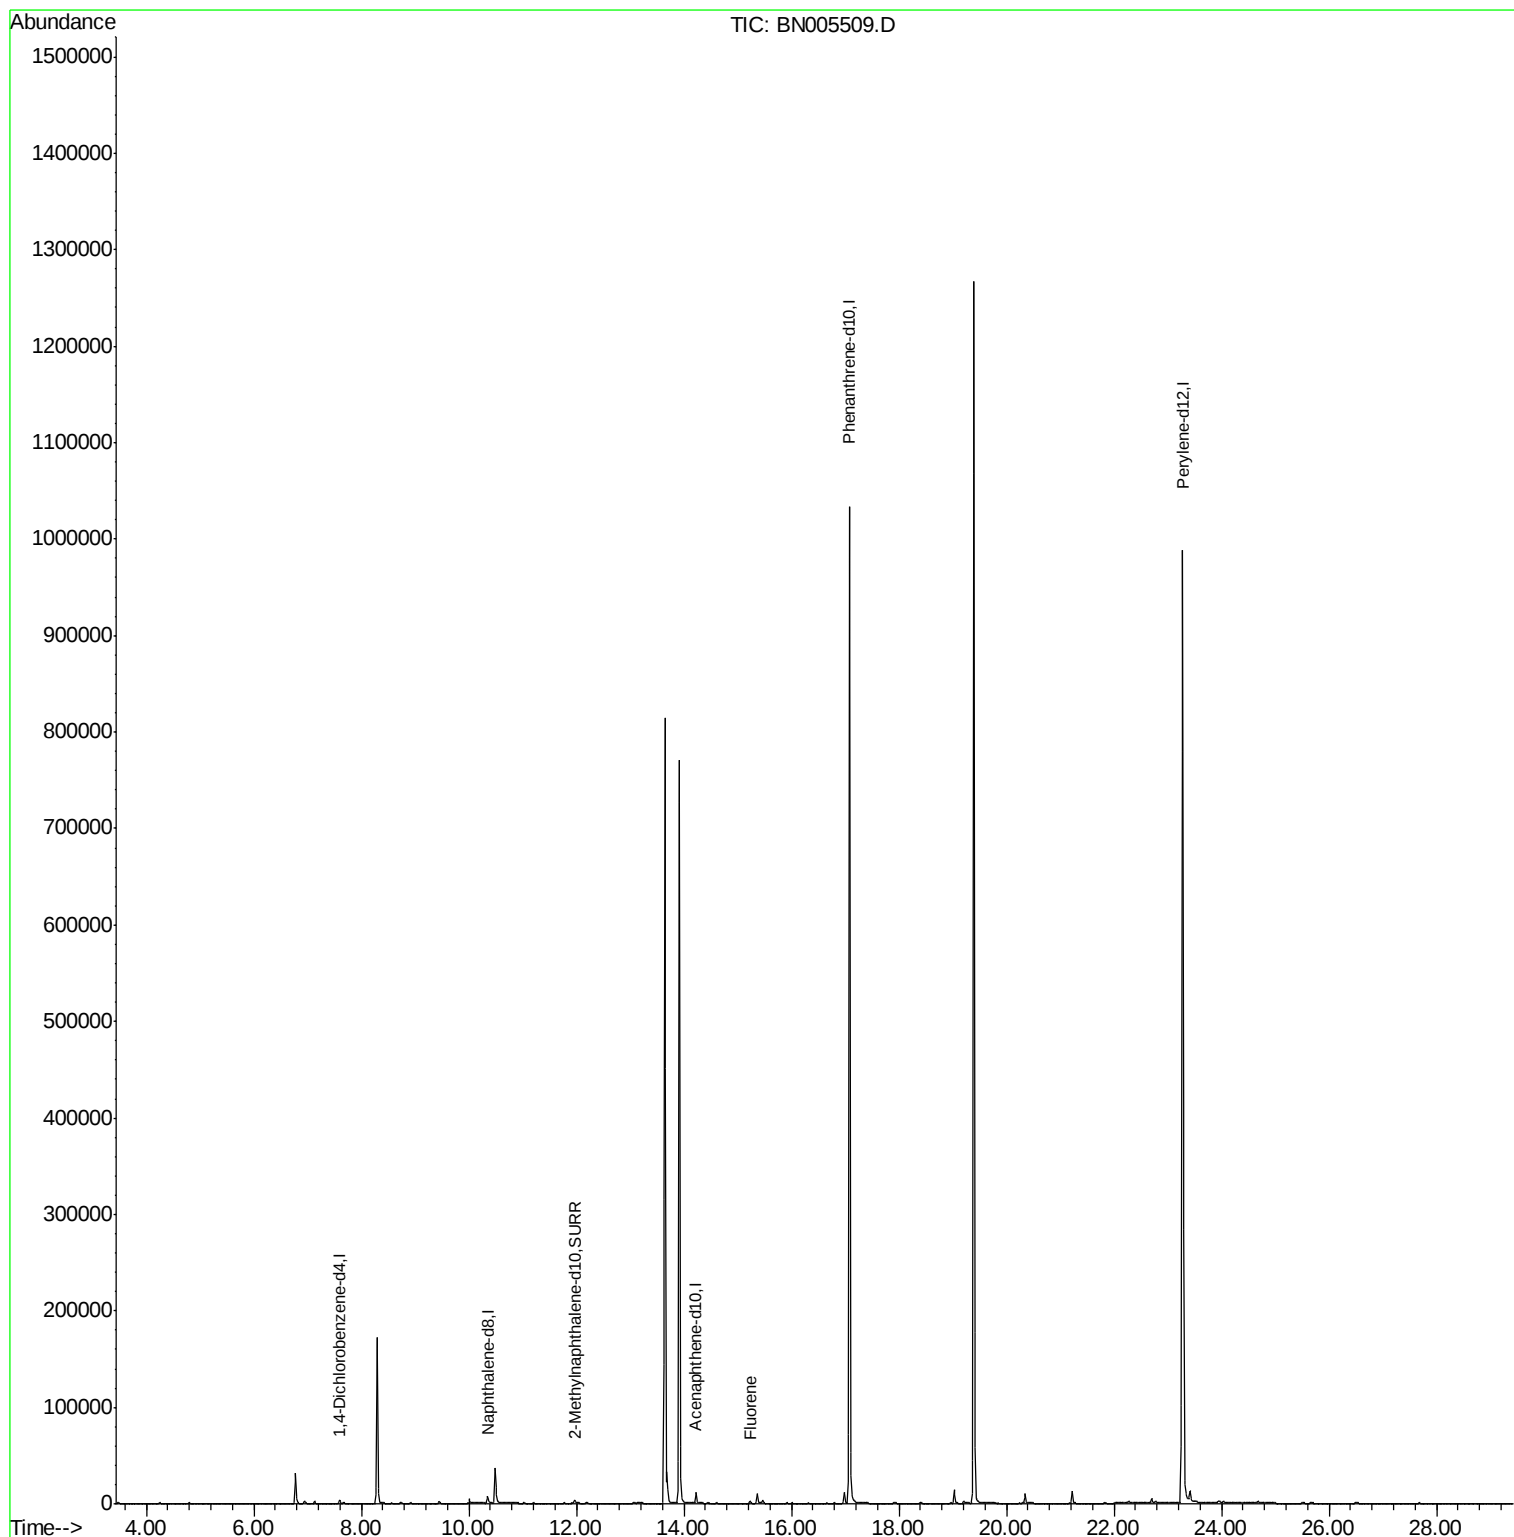

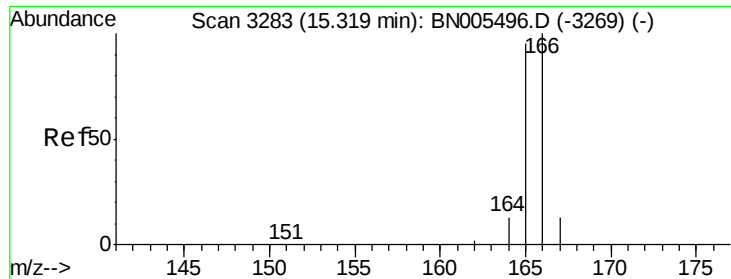

#9

Fluorene

Concen: 0.077 ng/ul

RT: 15.23 min Scan# 3263

Delta R.T. -0.09 min

Lab File: BN005509.D

Acq: 07 May 2019 05:05

Instrument :

BNA_N

ClientSampleId :

A5127



Tgt Ion:166 Resp: 1937

Ion Ratio Lower Upper

166 100

165 9.1 78.0 117.0#

167 35.7 12.2 18.4#

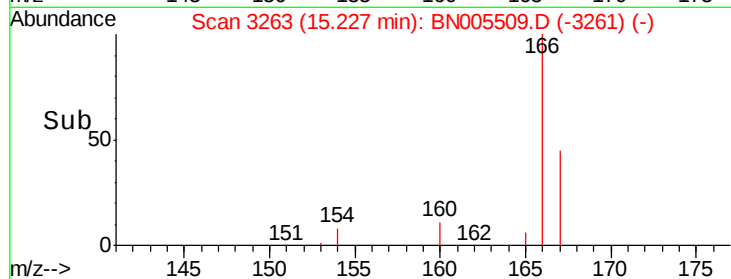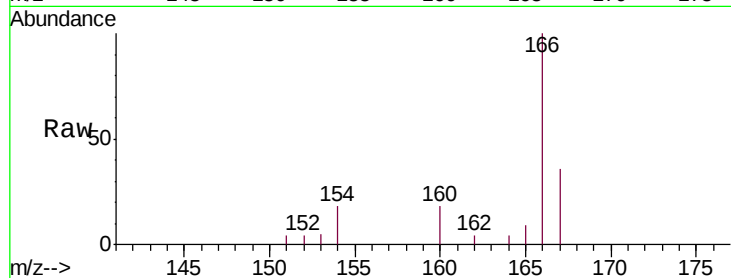

Abundance Ion 166.00 (165.70 to 166.70): E

2000 Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

